


MASS SPECTROMETRY REPORT

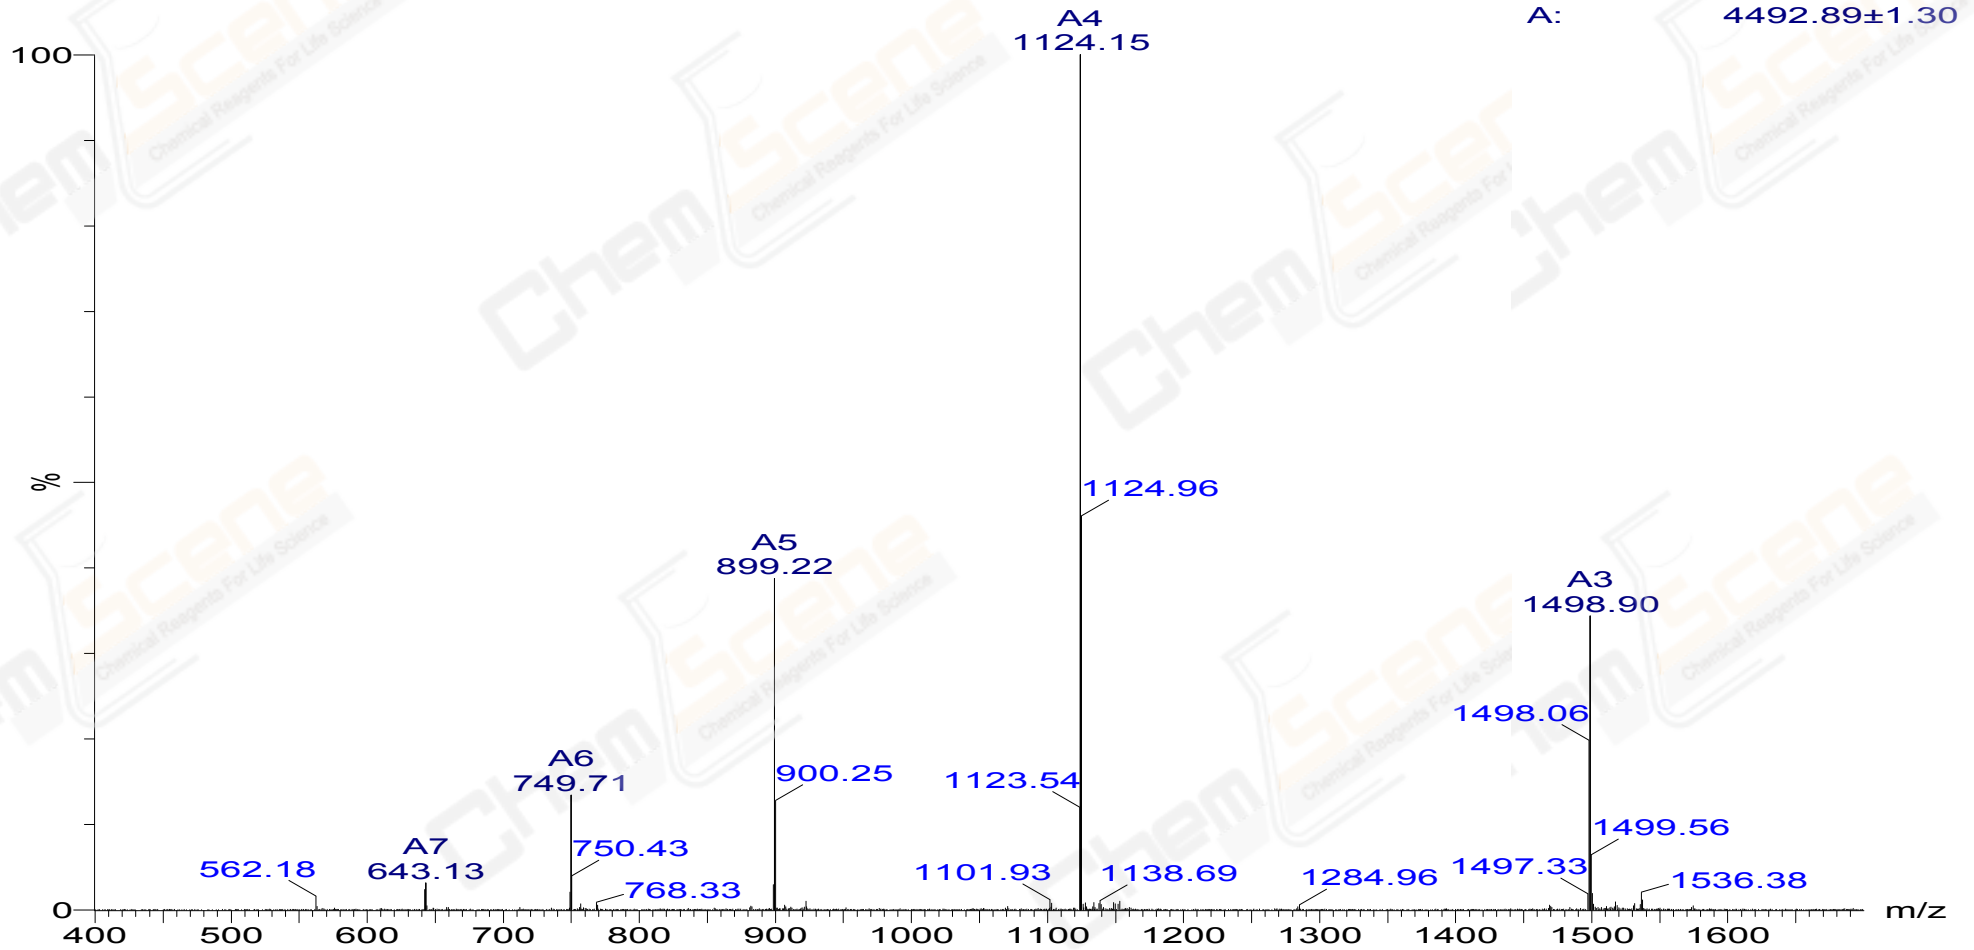

A: 4492.89±1.30

Sample Description

Analyzed date: 2022-06-09
Analyst: SHAO
Sample: 800072
M.W.: 4493.3
Product Name: LL-37, human (TFA)

Instrument

Probe: ESI
Nebulizer Gas Flow: 1.5L/min
CDL: -20.0v
CDL Temp.: 250 °C
Block Temp.: 200 °C

SHIMADZU LCMS-2020

Probe Bias: +4.5kv
Detector: 1.5kv
T. Flow: 0.2ml/min
B. Conc.: 50%H2O/50%ACN