


Product Name: NLS-StAx-h (TFA)

MASS SPECTROMETRY REPORT

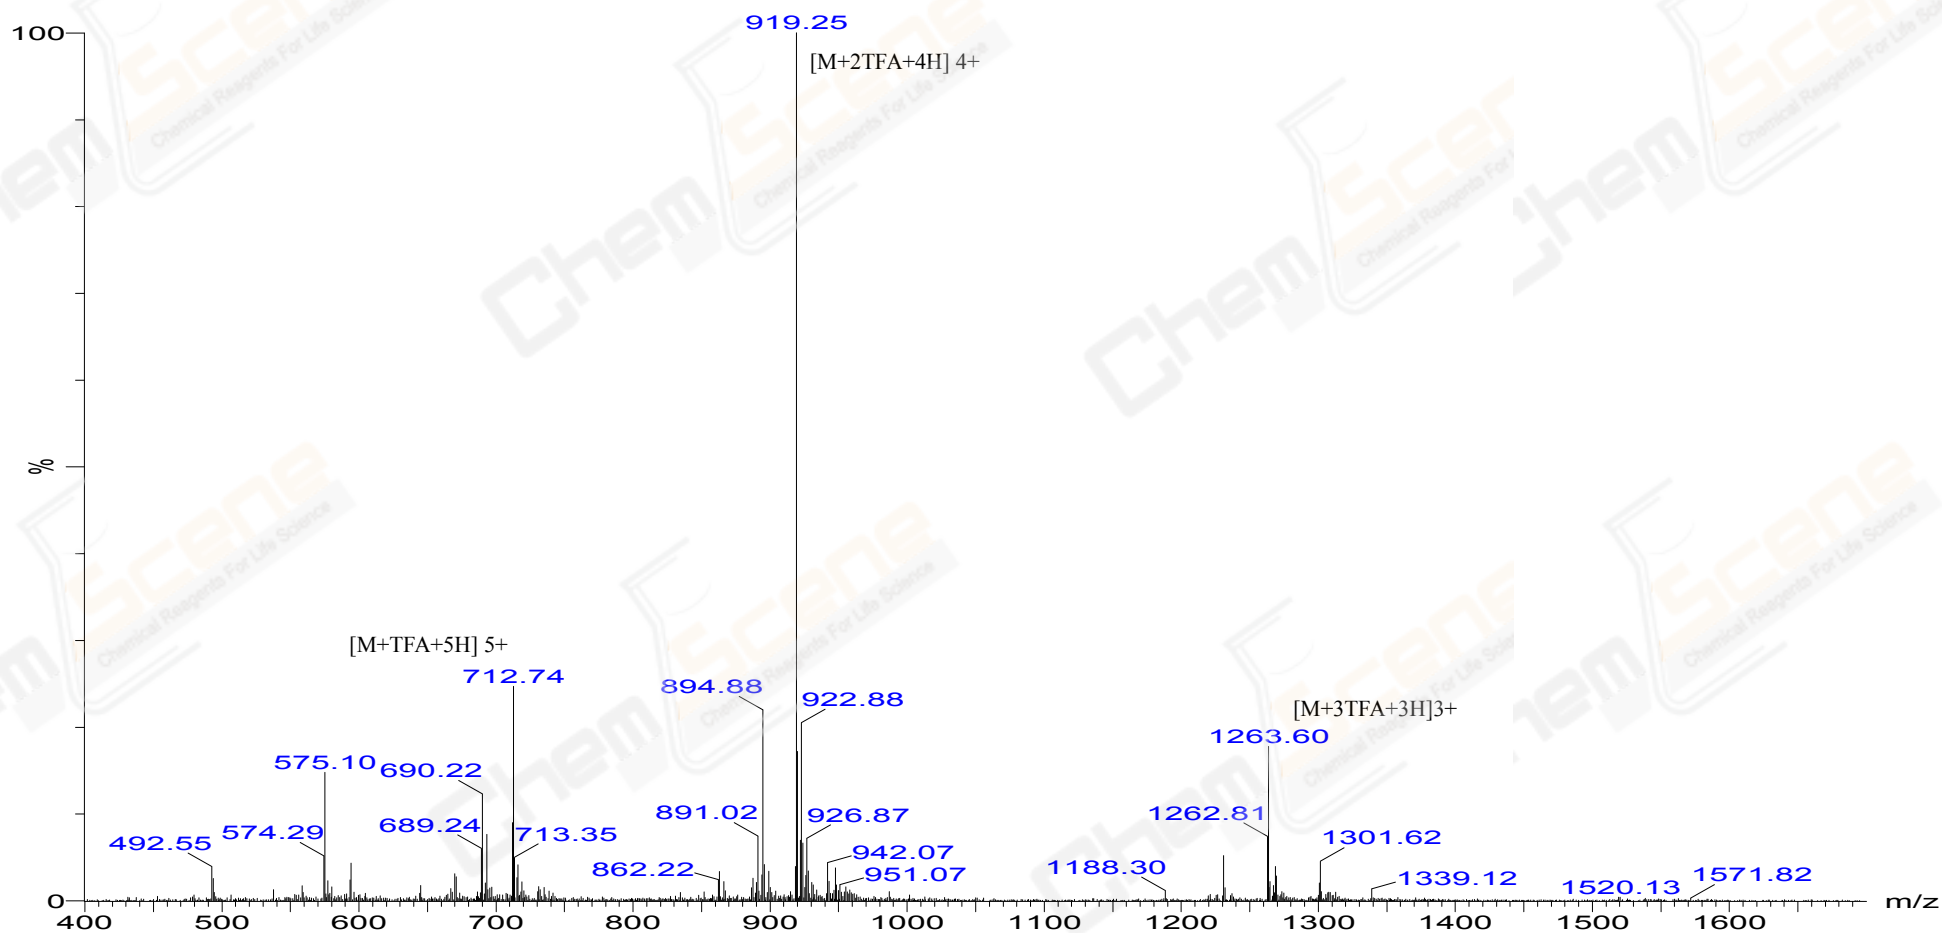

Sample Description

Analyzed date: 2021-10-18
Analyst: SHAO
Sample: 603193
M.W.: 3445.3
Lot. No.:

Instrument

Probe: ESI
Nebulizer Gas Flow: 1.5L/min
CDL: -20.0v
CDL Temp.: 250 °C
Block Temp.: 200 °C

SHIMADZU LCMS-2020

Probe Bias: +4.5kv
Detector: 1.5kv
T. Flow: 0.2ml/min
B. Conc.: 50%H2O/50%ACN