


# MASS SPECTROMETRY REPORT

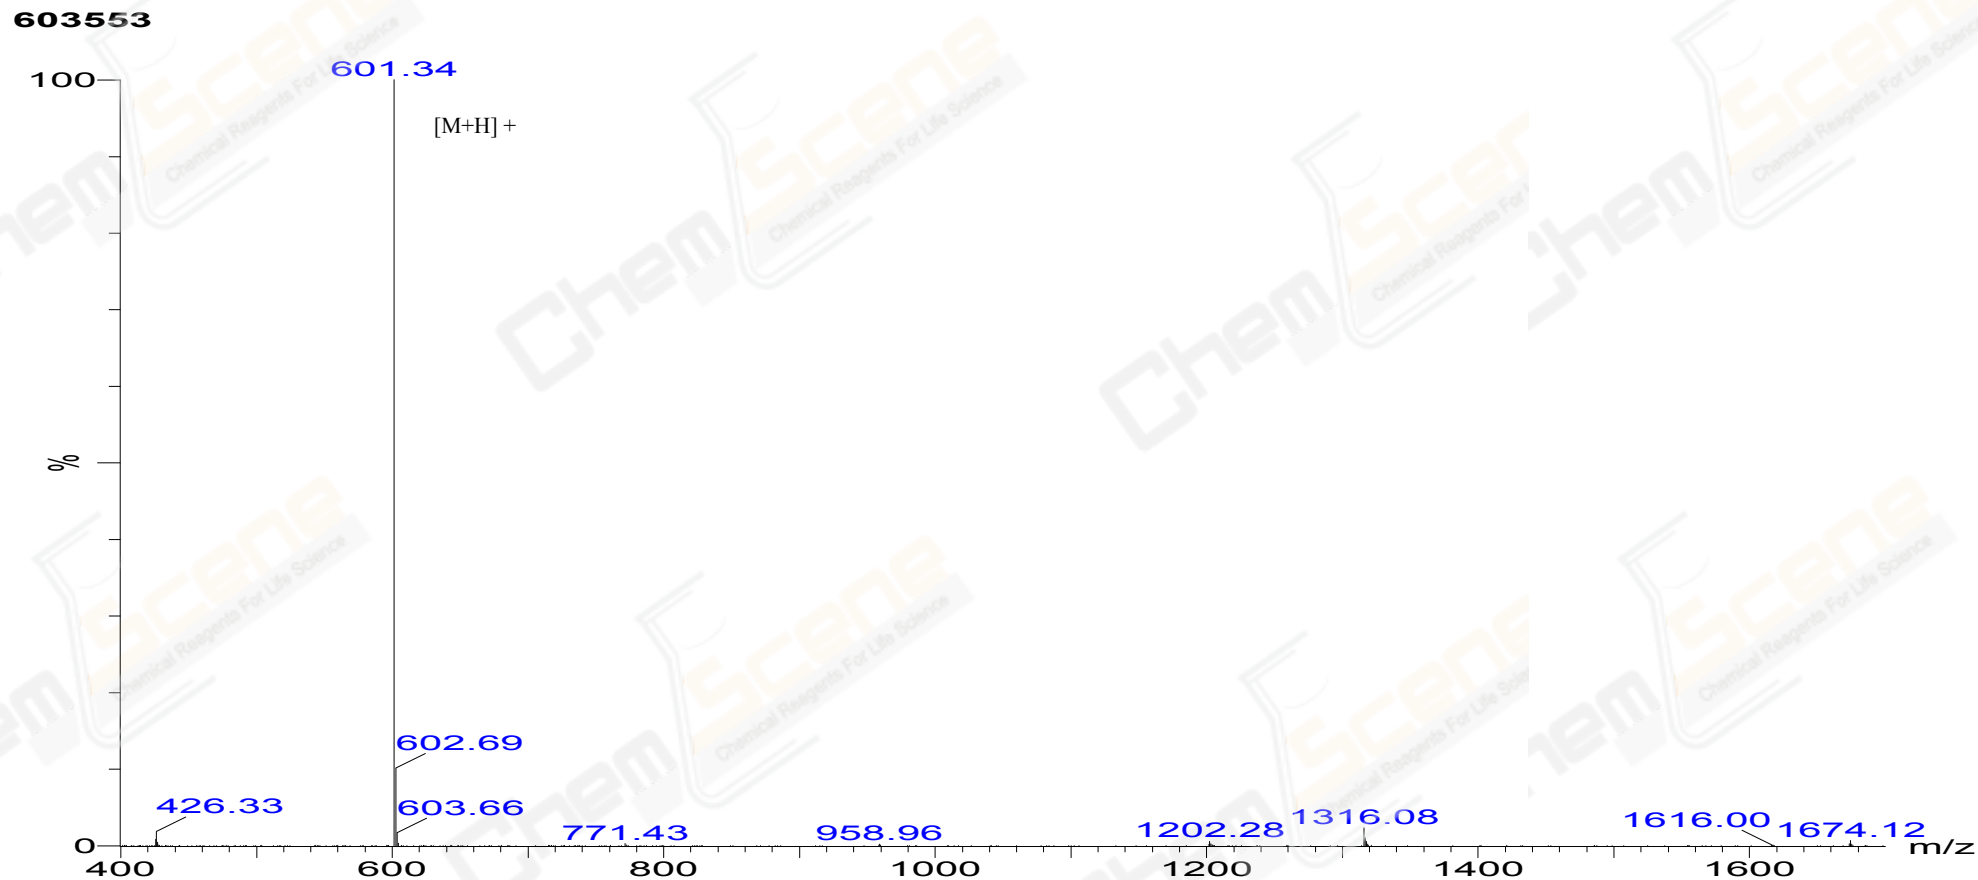

## Sample Description

Analyzed date: 2023-06-06  
Analyst: SHAO  
Sample: 603553  
M.W.: 600.7  
CAS NO.: 660846-97-9

## Instrument

Waters 2695  
Probe: ESI  
Nebulizer Gas Flow: 1.5L/min  
CDL: -20.0v  
CDL Temp.: 250 °C  
Block Temp.: 200 °C

Probe Bias: +4.5kv  
Detector: 1.5kv  
T. Flow: 0.5ml/min  
B. Conc.: 50%H<sub>2</sub>O/50%ACN