


MASS SPECTROMETRY REPORT

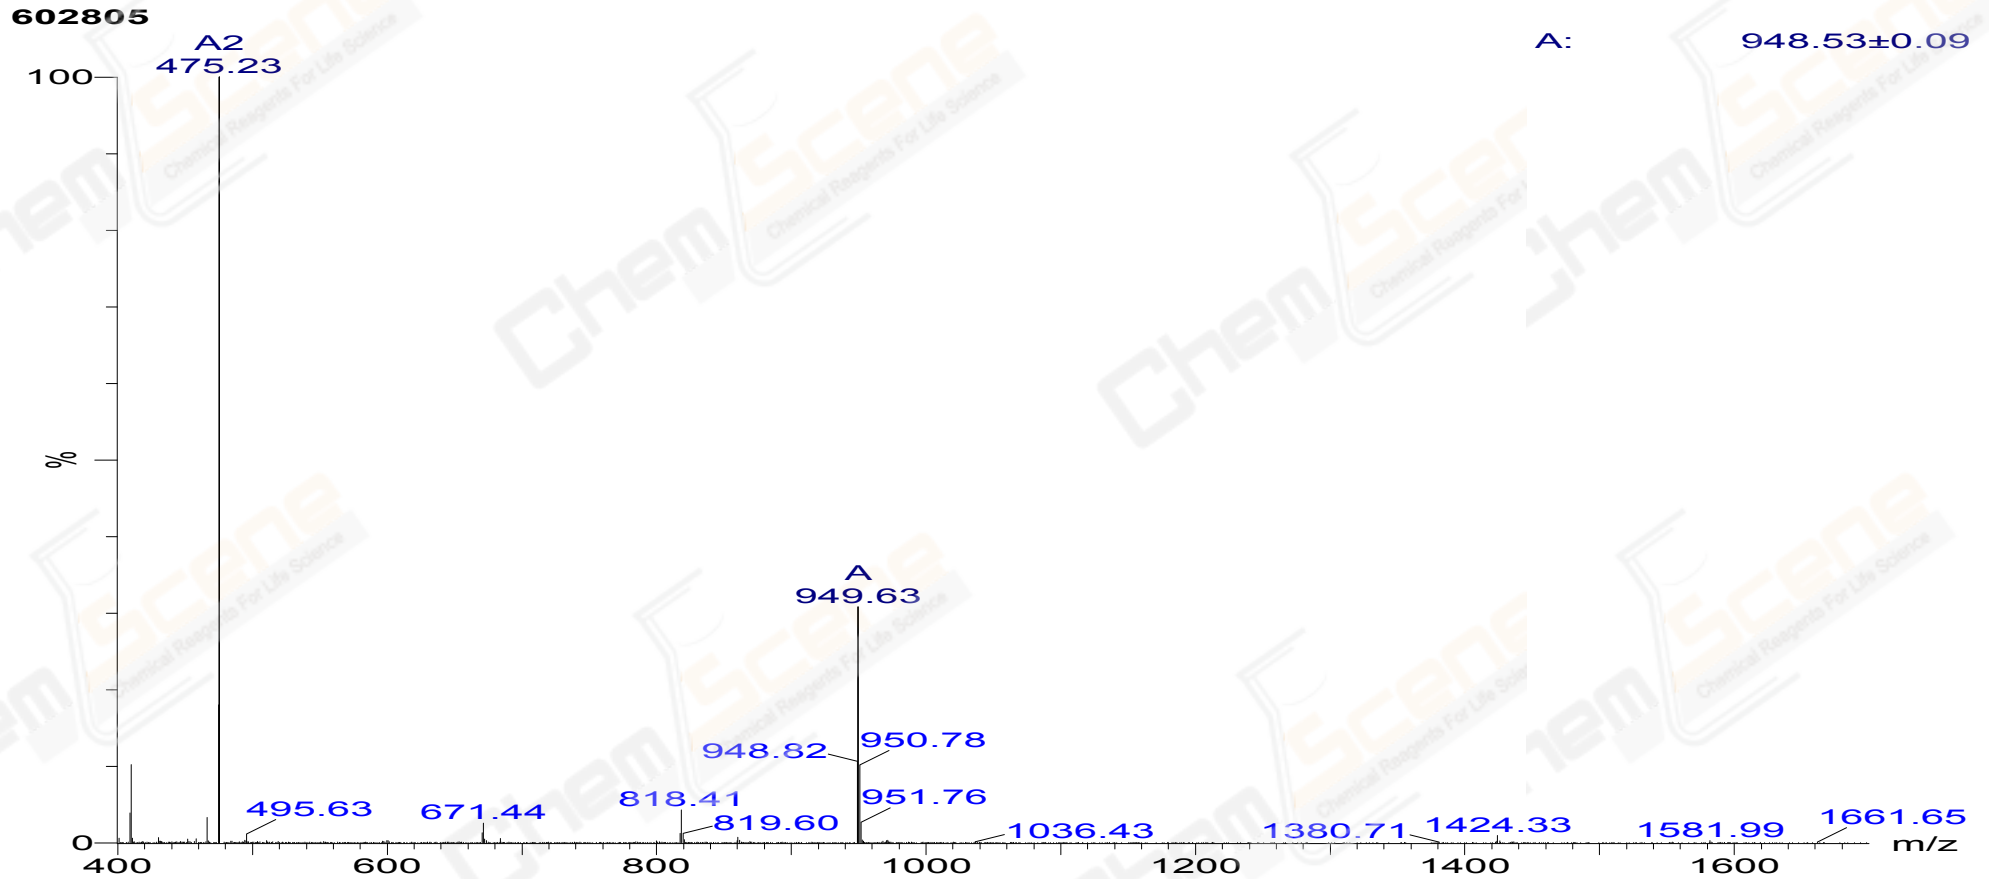

Sample Description

Analyzed date: 2023-03-27
Analyst: SHAO
Sample: 602805
M.W.: 949.1
Product Name: Shepherdin (79-87) (TFA)

Instrument

Waters 2695
Probe: ESI
Nebulizer Gas Flow: 1.5L/min
CDL: -20.0v
CDL Temp.: 250 °C
Block Temp.: 200 °C

Probe Bias: +4.5kv
Detector: 1.5kv
T. Flow: 0.5ml/min
B. Conc.: 50%H2O/50%ACN