


# MASS SPECTROMETRY REPORT

601413

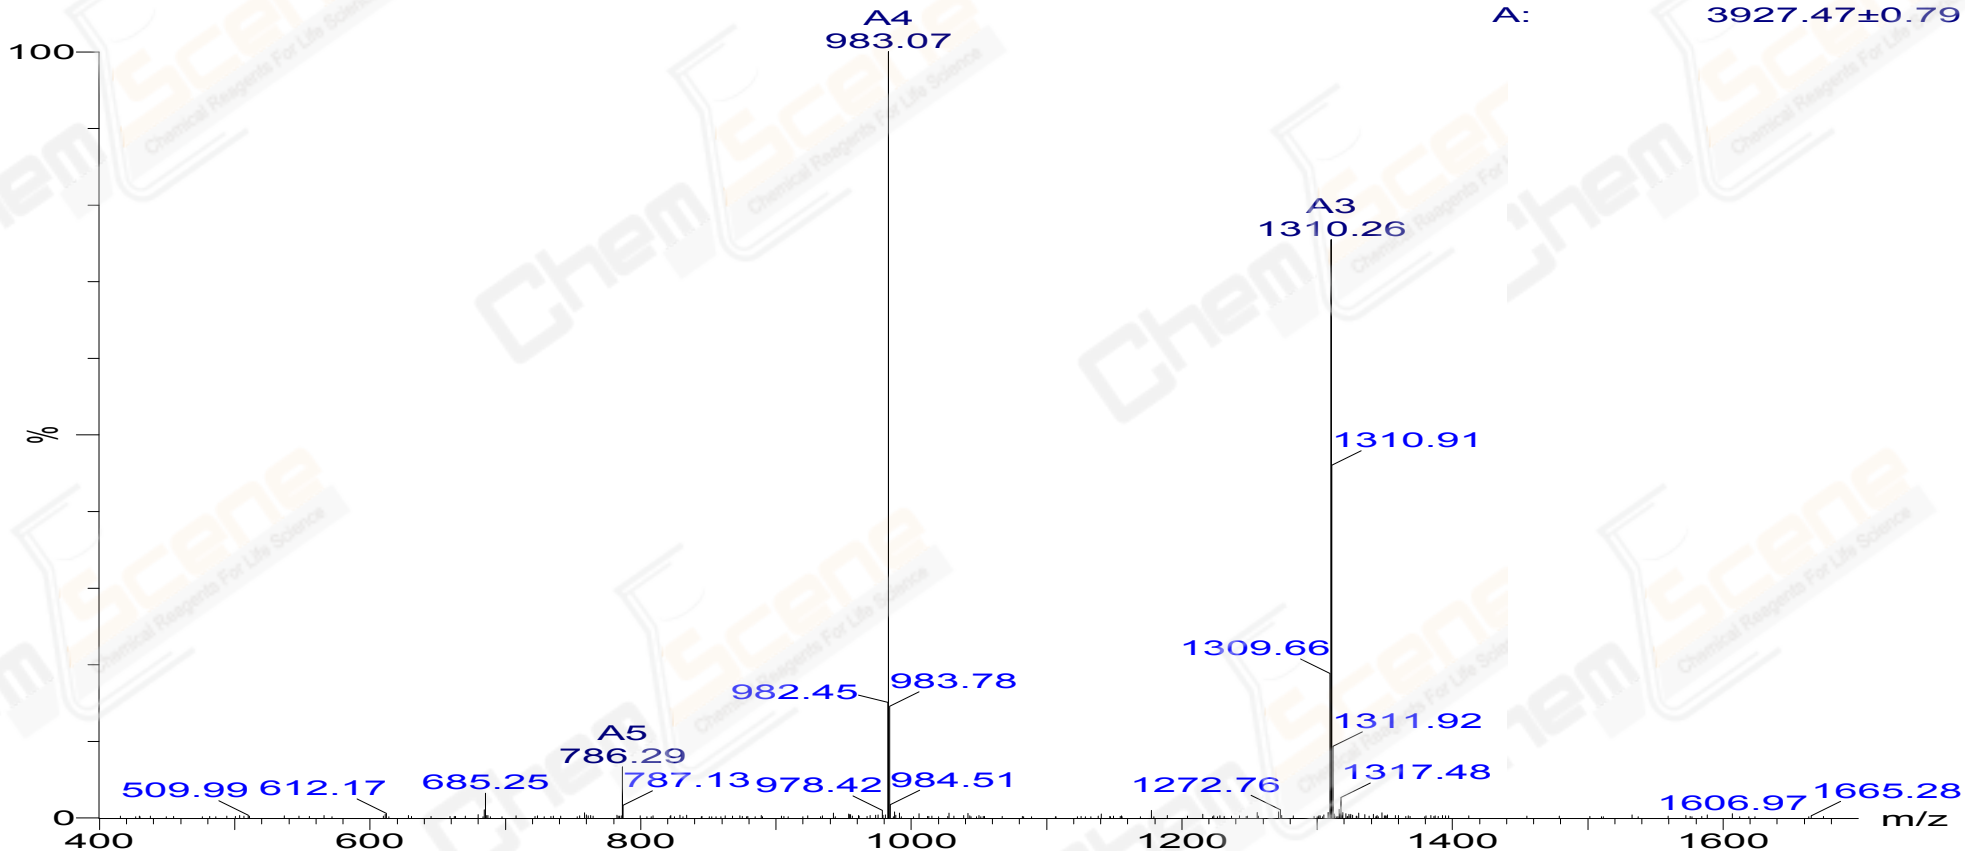

## Sample Description

Analyzed date: 2023-06-19  
Analyst: SHAO  
Sample: 601413  
M.W.: 3928.6  
CAS NO.: 452274-53-2

## Instrument

Waters 2695  
Probe: ESI  
Nebulizer Gas Flow: 1.5L/min  
CDL: -20.0v  
CDL Temp.: 250 °C  
Block Temp.: 200 °C

## Probe Bias:

+4.5kv  
Detector: 1.5kv  
T. Flow: 0.5ml/min  
B. Conc.: 50%H2O/50%ACN