


Product Name: LL-37, human (TFA)

### MASS SPECTROMETRY REPORT

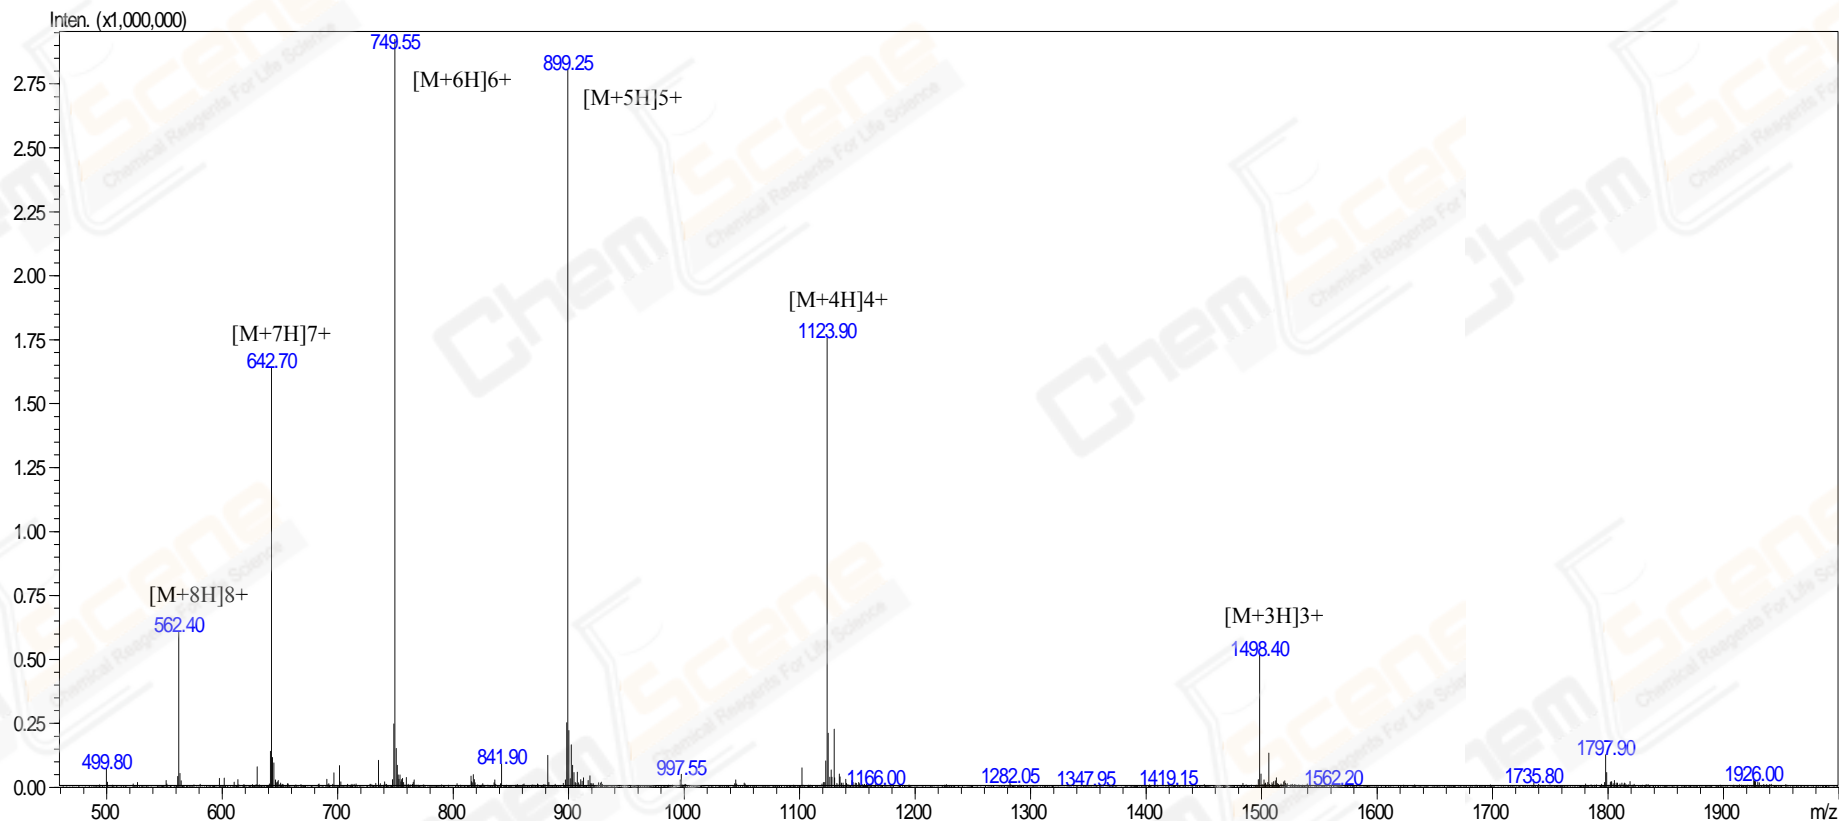

**Sample Description**

Analyzed date: 2019/6/29

Analyst: Shen

Sample: LL-37,Human LS-3 7

M.W.: 4493.26

**Instrument**

SHIMADZU LCMS-2020

**Probe:**

ESI

**Probe Bias:**

+4.5kv

**Nebulizer Gas Flow:**

1.5L/min

**Detector:**

1.2kv

**CDL:**

-20.0v

**T. Flow:**

0.2ml/min

**CDL Temp.:**

250 °C

**B. Conc.:**

50%H2O/50%ACN

Temp.: °C400