


Product Name: xStAx-VHLL

MASS SPECTROMETRY REPORT

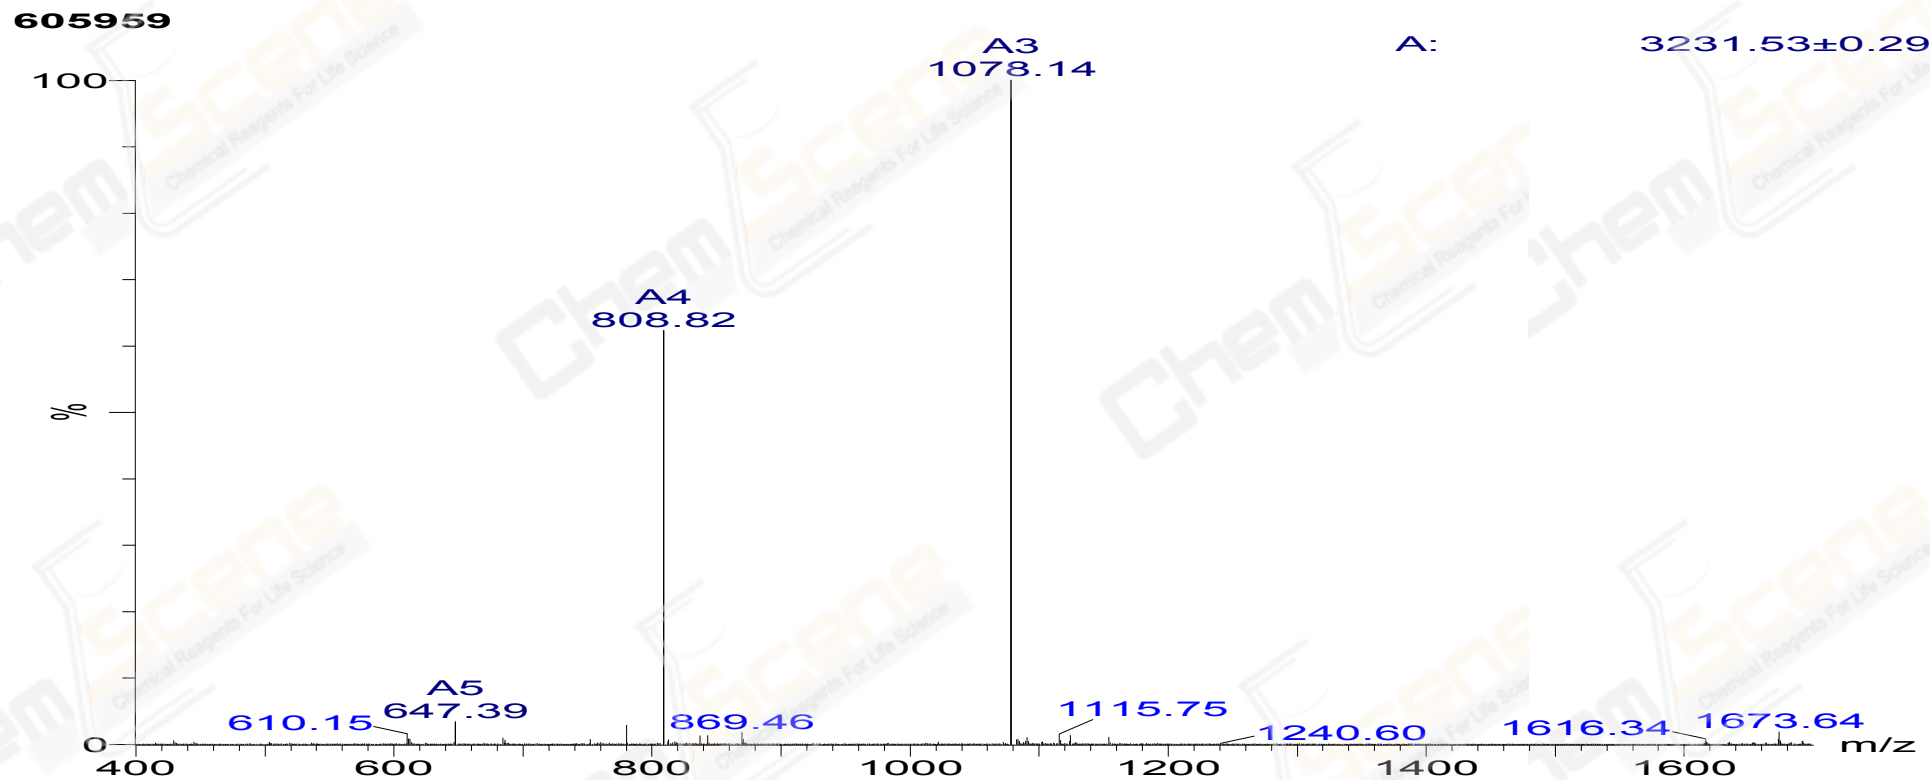

Sample Description

Analyzed date: 2024-07-26
Analyst: SHAO
Sample: 605959
M.W.: 3232.0
Lot. No.:

Instrument

Waters ZQ2000
Probe: ESI
Nebulizer Gas Flow: 10 L/min
CDL: 52.0v
CDL Temp.: 350 °C
Block Temp.: 120 °C

Probe Bias: +3.5kv
Detector: 0.05kv
T. Flow: 0.5ml/min
B. Conc.: 50%H2O/50%ACN