


MASS SPECTROMETRY REPORT

Product Name: NLS-StAx-h (TFA)

A: 3445.00±0.58

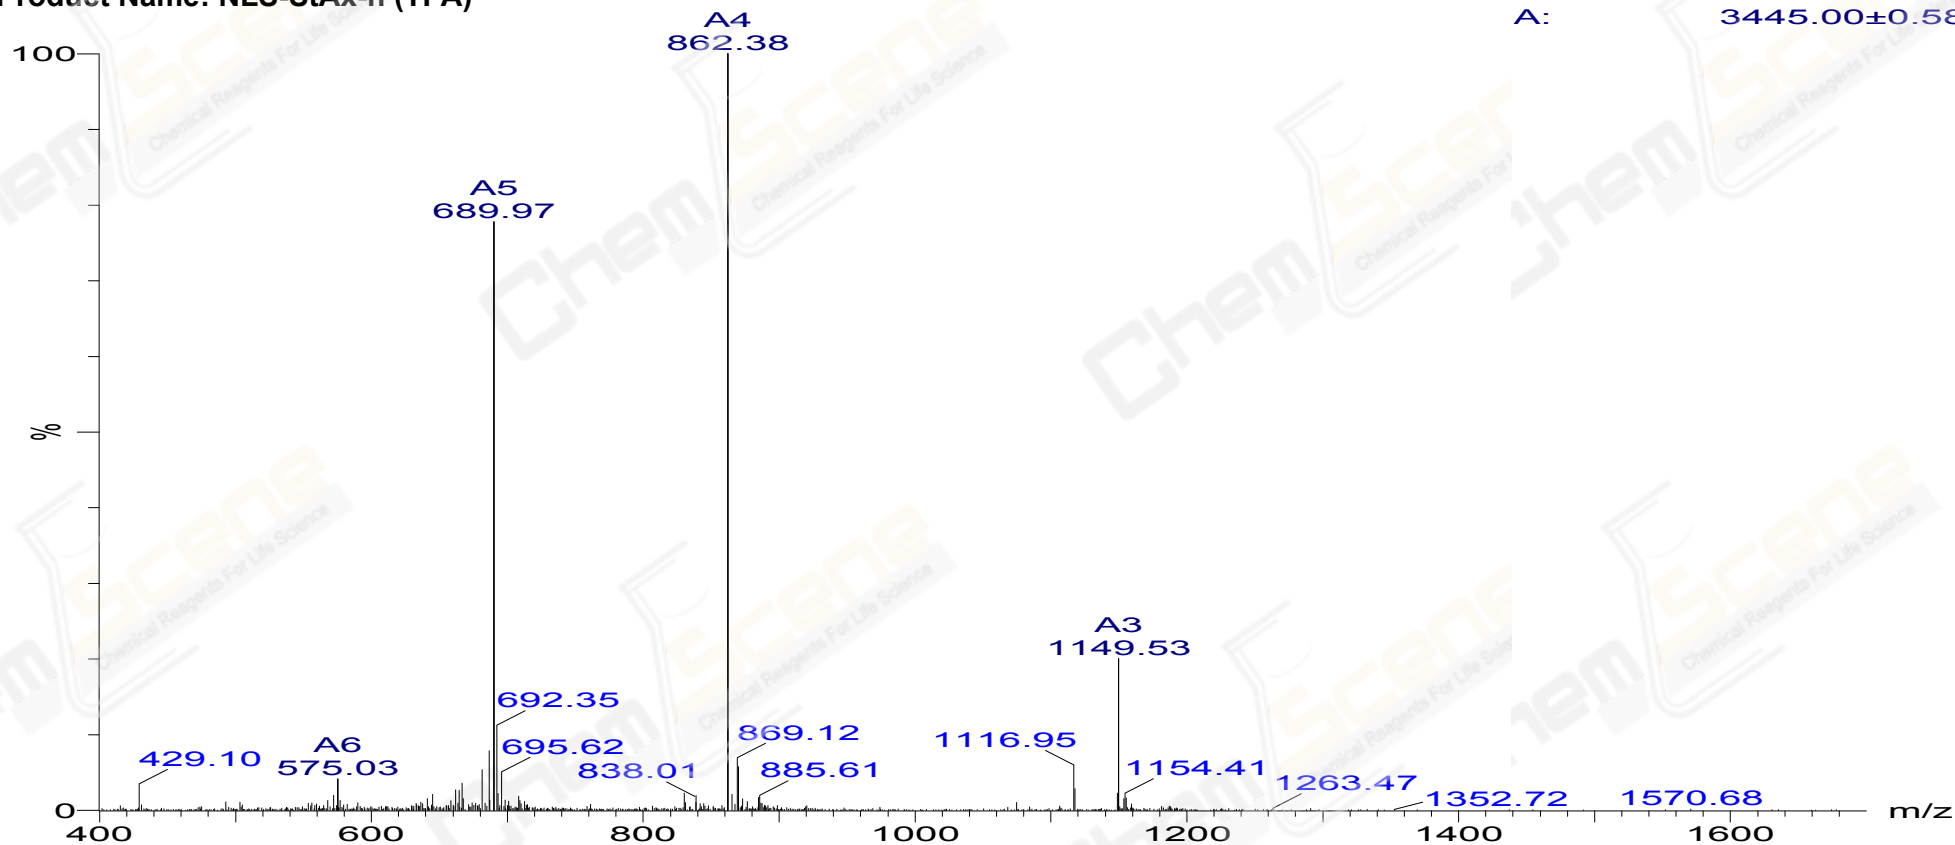

Sample Description

Analyzed date: 2023-12-07
Analyst: SHAO
Sample: 603193
M.W.: 3445.3

Instrument

Waters 2695
Probe: ESI
Nebulizer Gas Flow: 1.5L/min
CDL: -20.0v
CDL Temp.: 250 °C
Block Temp.: 200 °C

Probe Bias: +4.5kv
Detector: 1.5kv
T. Flow: 0.5ml/min
B. Conc.: 50%H2O/50%ACN