


MASS SPECTROMETRY REPORT

602803

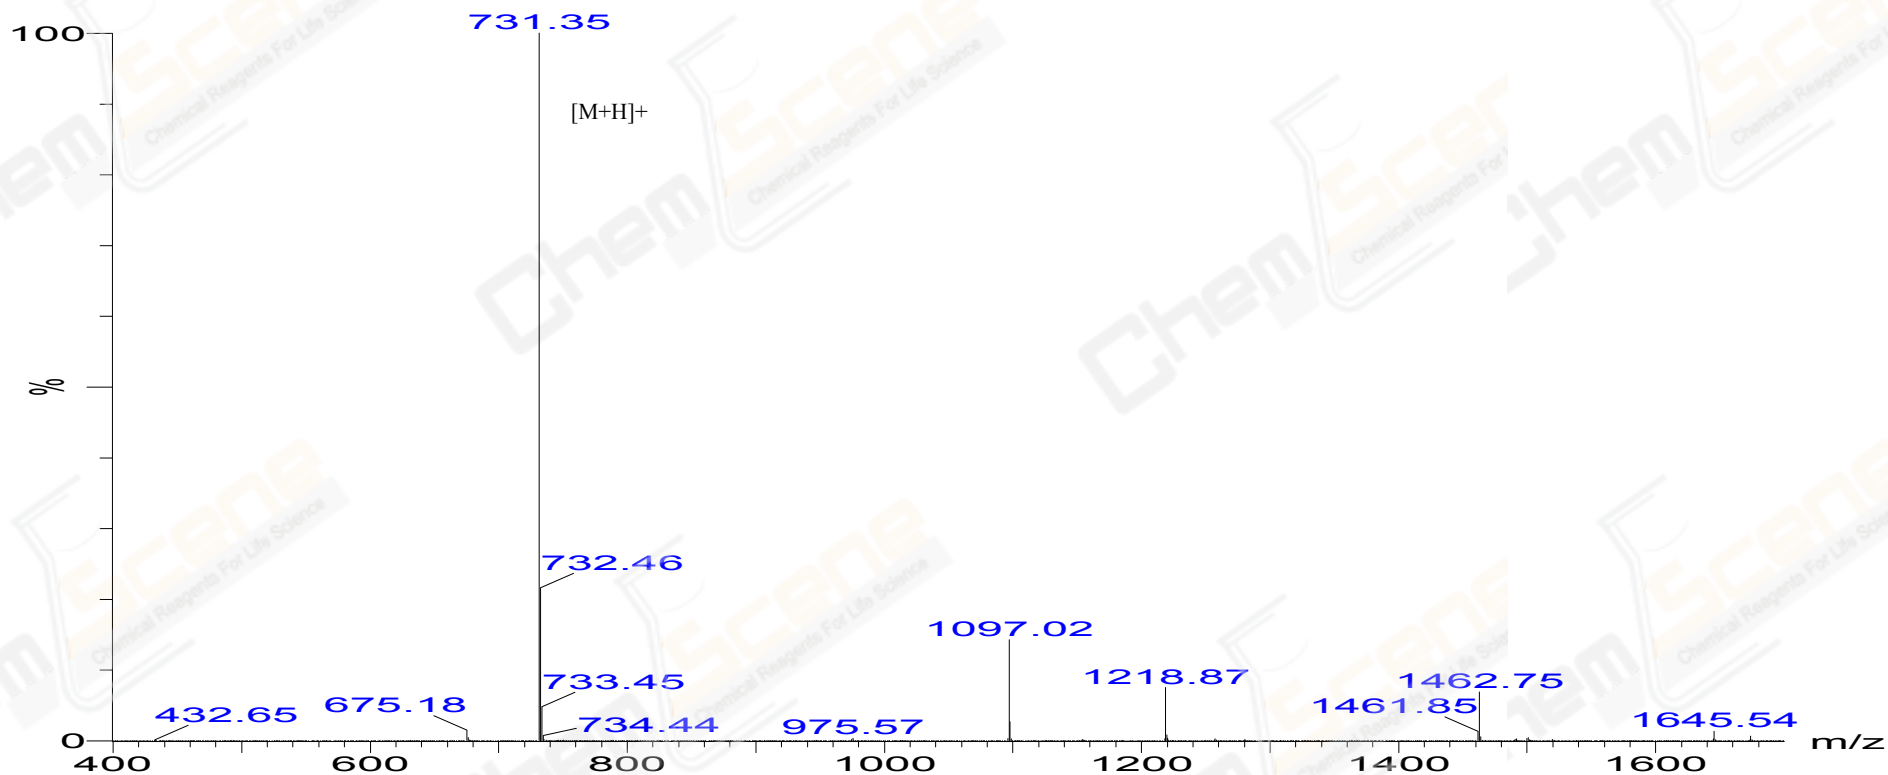

Sample Description

Analyzed date: 2024-11-11
Analyst: SHAO
Sample: 602803
M.W.: 730.8
CAS NO.: 65147-06-0

Instrument

Waters ZQ 2000
Probe: ESI
Nebulizer Gas Flow: 10L/min
CDL: 52.0v
CDL Temp.: 350 °C
Block Temp.: 120 °C

Probe Bias:

+3.5kv

Detector:

0.05kv

T. Flow:

0.5ml/min

B. Conc.:

50%H₂O/50%ACN