


525MS

Sample Name:		Injection Volume:	1.0
Vial Number:	GA7	Channel:	UV_VIS_1
Sample Type:	unknown	Mass Range:	n.a.
Control Program:	PH-45V	Polarity:	n.a.
Quantif. Method:	AAA	Dilution Factor:	1.0000
Recording Time:	1/24/2014 9:12	Sample Weight:	1.0000
Run Time (min):	2.50	Sample Amount:	1.0000

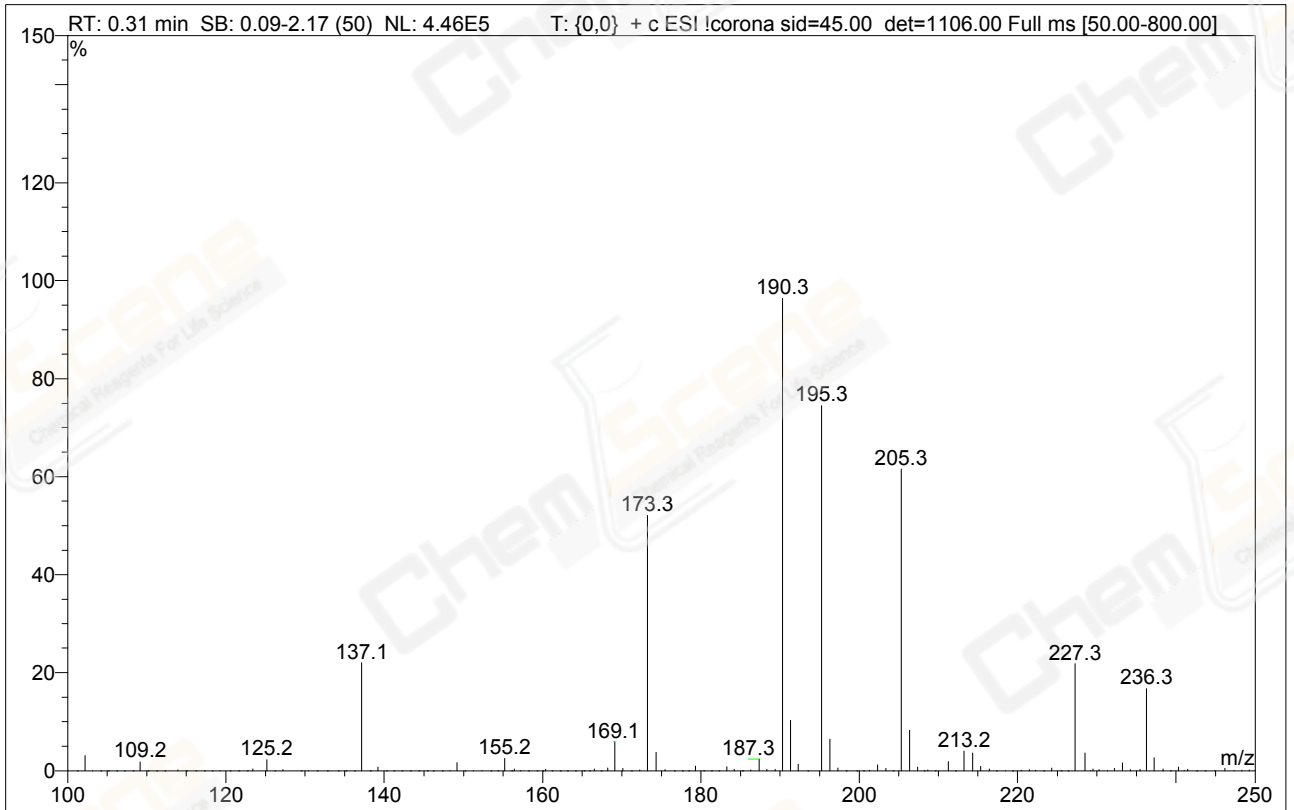

No.	Ret.Time min	Peak Name	Base Peak Int. amu	Peak 1 amu	Peak 2 amu	Peak 3 amu	Int. Peaks delta%
Average delta% from expected Intensity:							n.a.