
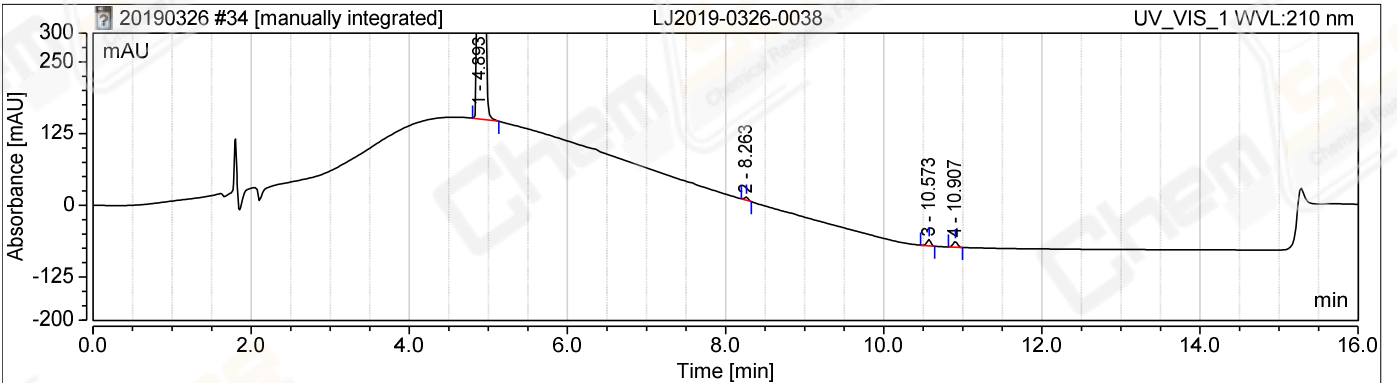


### Chromatogram and Results

#### Injection Details

Catalog No: <b>CS-W004546 Batch#Lc0326026</b>	Run Time (min): <b>16.00</b>
Vial Number: <b>GB3</b>	Users: <b>zqq</b>
Injection Type: <b>Unknown</b>	Injection Volume: <b>5.00</b>
Calibration Level:	Channel: <b>UV_VIS_1</b>
Instrument Method: <b>10-90A 214NM</b>	Wavelength: <b>210</b>
Processing Method: <b>3D Quantitative</b>	Bandwidth: <b>4</b>
Comment: <b>1053534 A-RP-328</b>	Dilution Factor: <b>1.0000</b>
Injection Date/Time: <b>26/Mar/19 22:19</b>	Sample Weight: <b>1.0000</b>

#### Chromatogram

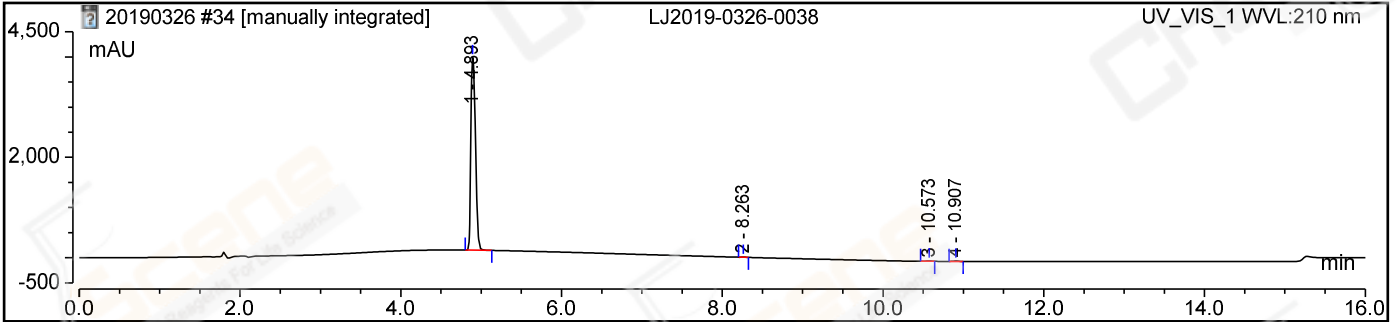

#### Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Resolution (EP)	Match	Asymmetry (EP)	Rel.Area %
1		4.893	256.307	3840.021	35.32	957	1.42	99.40
2		8.263	0.285	5.564	26.53	888	1.01	0.11
3		10.573	0.636	10.805	3.46	965	0.91	0.25
4		10.907	0.638	9.985	n.a.	994	0.93	0.25
<b>Total:</b>			<b>257.866</b>	<b>3866.375</b>	<b>65.31</b>			<b>4.27</b>