
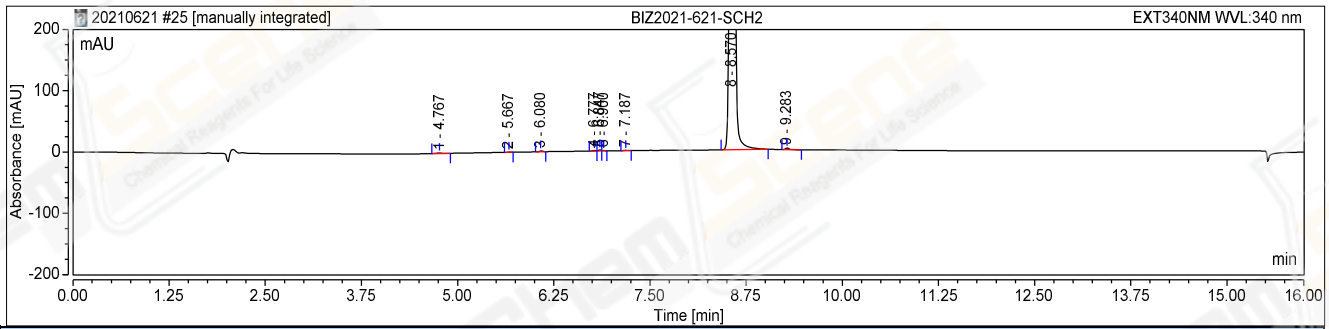


Chromatogram and Results

Injection Details

Injection Name: BIZ2021-621-SCH2	Run Time (min): 16.00	
Vial Number: RB6	Injection Volume: 10.00	
Injection Type: Unknown	Channel: EXT340NM	
User: zhangqingqing	Wavelength: n.a.	
Instrument Method: 10-90A 214NM	Bandwidth: n.a.	
Processing Method: 3D Quantitative	Dilution Factor: 1.0000	
Injection Data/Time: 21/Jun/2021 18:36	Sample Weight: 1.0000	
Comment: 20210621 A-RP-760	Instrument Data\202106\20210621.seq	
chrom://hy637/ChromeleonLocal/Instrument Data/202106/20210621.seq/208.smp/EXT340NM.channel/EXT340NM.chm		

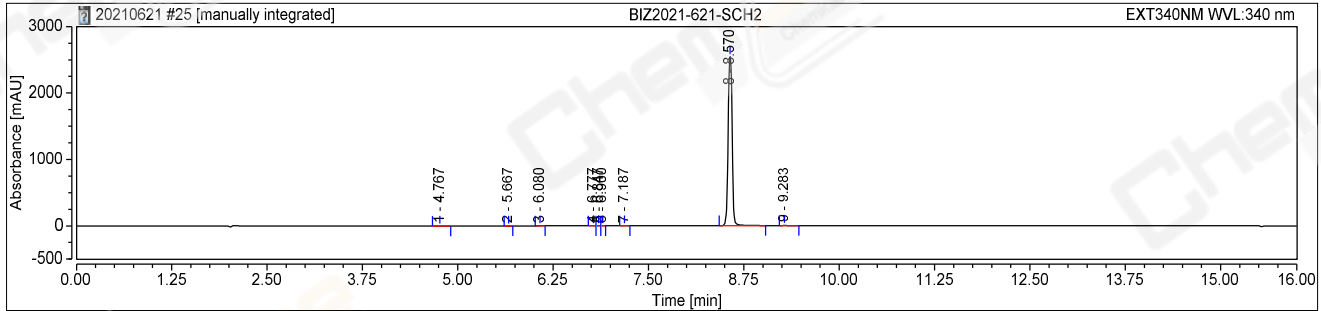

Integration Results

No.	Retention Time min	Area mAU*min	Height mAU	Resolution (USP)	Match	Asymmetry (EP)	Rel.Area %
1	4.767	0.053	0.585	8.73	958	1.16	0.03
2	5.667	0.020	0.555	6.76	975	1.04	0.01
3	6.080	0.069	1.662	11.19	991	1.24	0.05
4	6.777	0.034	0.917	1.22	962	n.a.	0.02
5	6.847	0.066	1.913	0.90	997	n.a.	0.04
6	6.900	0.035	0.955	4.03	997	n.a.	0.02
7	7.187	0.027	0.532	16.69	994	1.08	0.02
8	8.570	153.172	2543.137	8.81	979	1.01	99.72
9	9.283	0.122	2.491	n.a.	900	1.05	0.08
Total:	153.597	2552.747	58.33	6.58			