
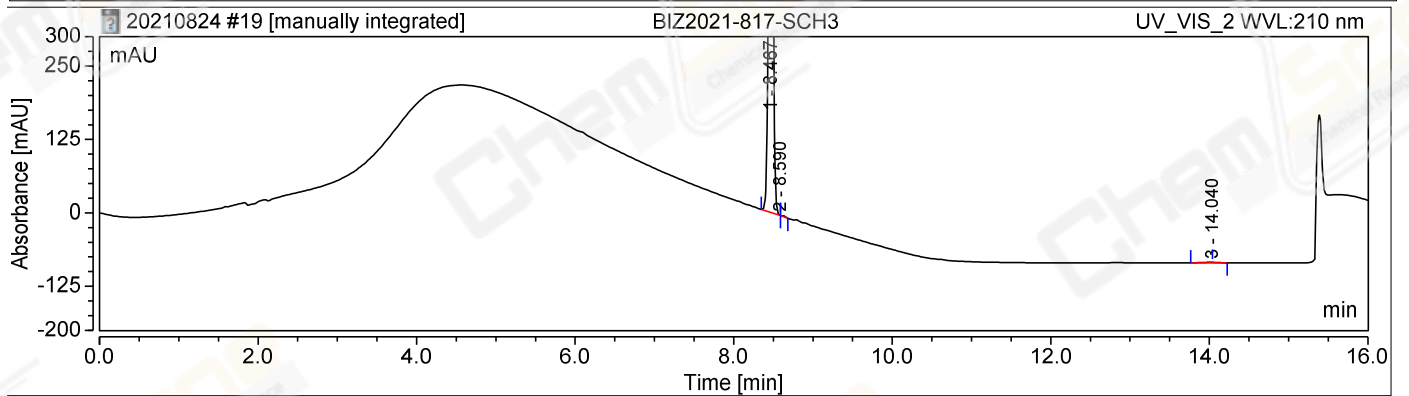


Chromatogram and Results

Injection Details		
Injection Name:	BIZ2021-817-SCH3	Run Time (min): 16.00
Vial Number:	RC8	Users: liyan
Injection Type:	Unknown	Injection Volume: 1.00
Calibration Level:		Channel: UV_VIS_2
Instrument Method:	10-90A,214NM	Wavelength: 210
Processing Method:	3D Quantitative	Bandwidth: 4
CAS NO.:	256373-96-3 A-RP-537	Dilution Factor: 1.0000
Injection Date/Time:	24/Aug/21 19:18	Sample Weight: 1.0000
chrom://hy442/DATA2/Instrument Data/202108/20210824.seq/636.smp/UV_VIS_2.channel/UV_VIS_2.chm		

Chromatogram

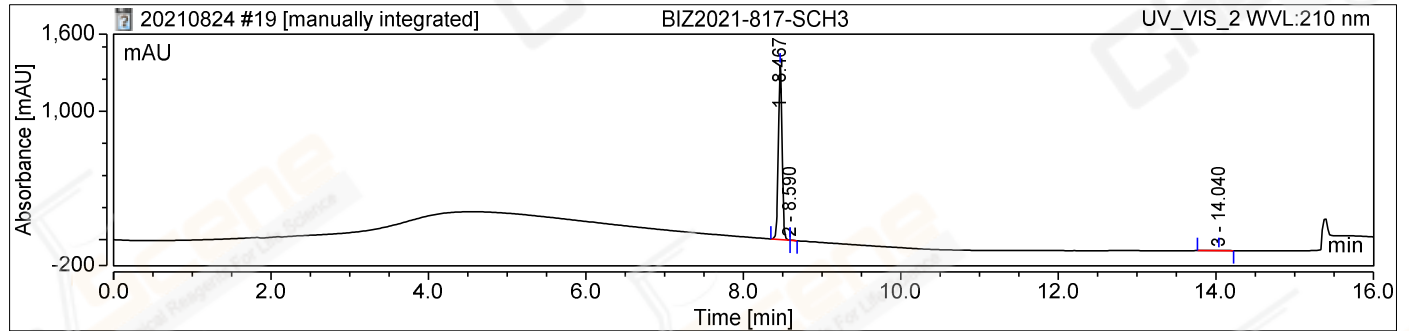

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Match	Resolution (EP)	Asymmetry (EP)	Rel.Area %
1		8.467	73.088	1353.666	1000	n.a.	1.01	99.61
2		8.590	0.070	0.000	1000	n.a.	n.a.	0.10
3		14.040	0.218	0.966	817	n.a.	0.84	0.30
Total:			73.376	1354.632			0.00	1.85