



## Chromatogram and Results

### Injection Details

<b>Injection Name:</b> BIZ2021-819-SCH6	<b>Run Time (min):</b> 16.00
<b>Vial Number:</b> RC2	<b>Users:</b> liyan
<b>Injection Type:</b> Unknown	<b>Injection Volume:</b> 2.00
<b>Calibration Level:</b>	<b>Channel:</b> UV_VIS_1
<b>Instrument Method:</b> 10-90A,214NM	<b>Wavelength:</b> 214
<b>Processing Method:</b> 3D Quantitative	<b>Bandwidth:</b> 4
<b>Comment:</b> A-RP-537	<b>Dilution Factor:</b> 1.0000
<b>Injection Date/Time:</b> 24/Aug/21 22:52	<b>Sample Weight:</b> 1.0000

**chrom://hy442/ATA2/Instrument Data/202108/20210824.seq/678.smp/UV\_VIS\_1.channel/UV\_VIS\_1.chm**

### Chromatogram

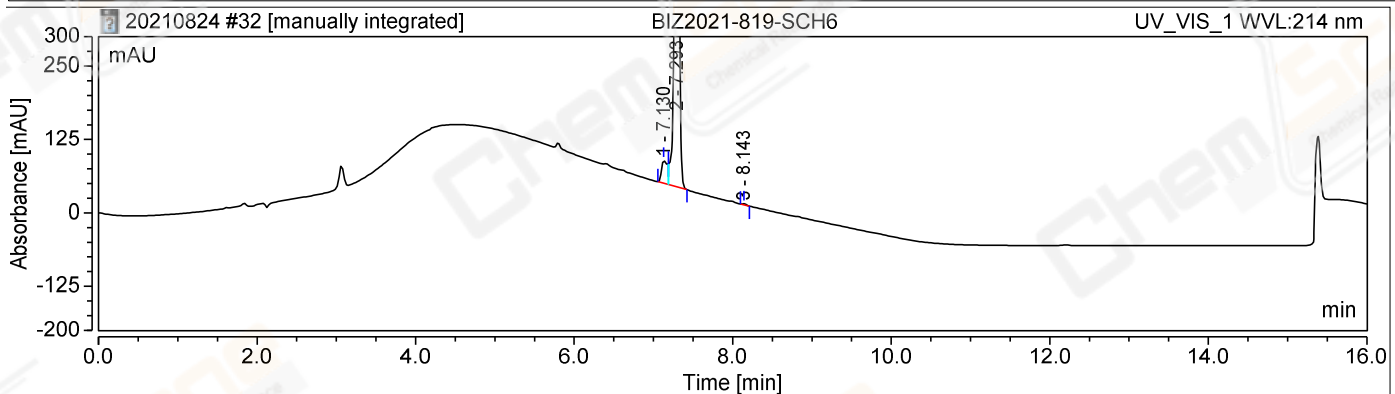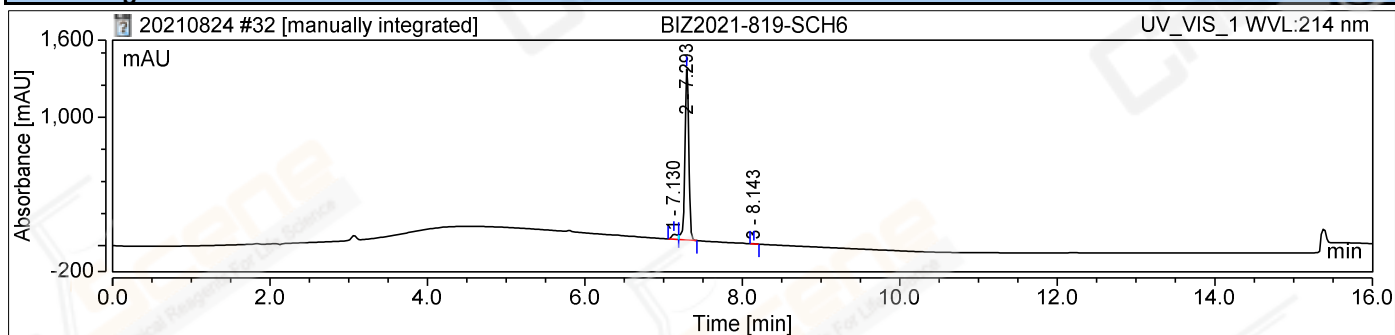

### Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Match	Resolution (EP)	Asymmetry (EP)	Rel.Area %
1		7.130	3.363	39.585	1000	n.a.	n.a.	4.39
2		7.293	73.058	1329.117	999	9.94	0.97	95.47
3		8.143	0.100	1.780	915	n.a.	1.23	0.13
<b>Total:</b>			<b>76.521</b>	<b>1370.482</b>			<b>9.94</b>	<b>2.21</b>