
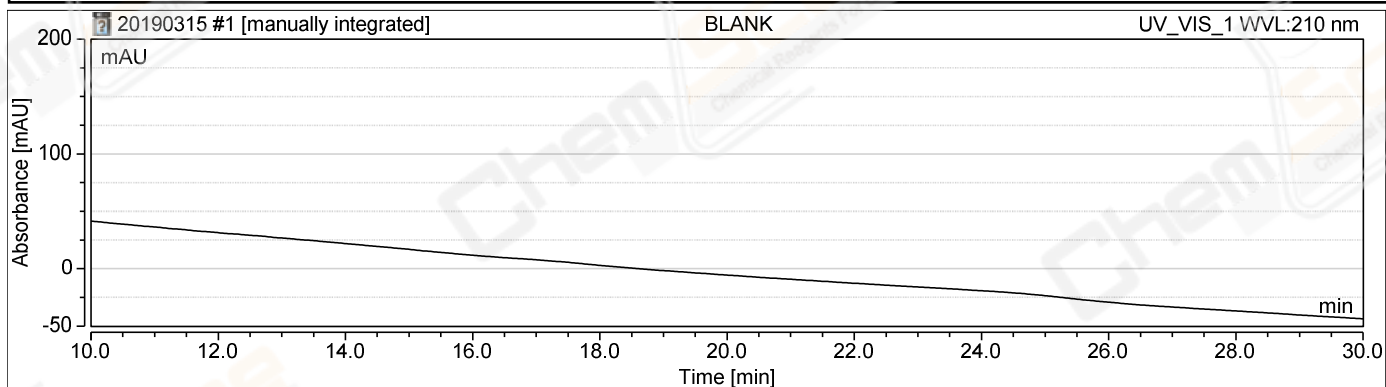


Chromatogram and Results

Injection Details

Injection Name:	BLANK	Run Time (min):	45.00
Vial Number:	RB5	Users:	zqq
Injection Type:	Unknown	Injection Volume:	5.00
Calibration Level:		Channel:	UV_VIS_1
Instrument Method:	HM-354_10A-H01P01.C2	Wavelength:	210
Processing Method:	New processing	Bandwidth:	4
Comment:	HM-345_10-20190314 Blank A-RP-126	Dilution Factor:	1.0000
Injection Date/Time:	15/Mar/19 10:56	Sample Weight:	1.0000

Chromatogram

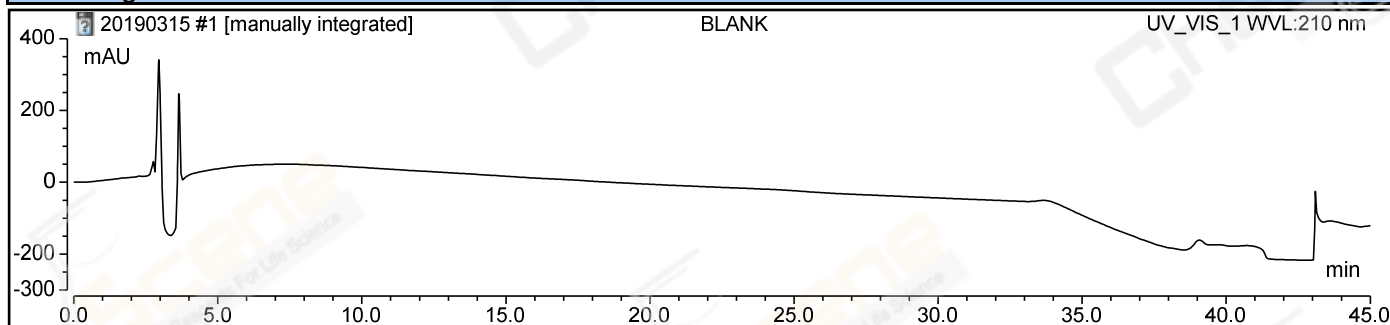

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Resolution (EP)	Match	Asymmetry (EP)	Rel.Area %
Total:			0.000	0.000	0.00			0.00



Chromatogram and Results

Injection Details

Injection Name: **CPK2019-314-12364**
 Vial Number: **RB6**
 Injection Type: **Unknown**
 Calibration Level:
 Instrument Method: **HM-354_10A-H01P01.C2**
 Processing Method: **New processing**
 Comment: **HM-345_10-20190314 A-RP-126**
 Injection Date/Time: **15/Mar/19 11:41**

Run Time (min): **45.00**
 Users: **zqq**
 Injection Volume: **5.00**
 Channel: **UV_VIS_1**
 Wavelength: **210**
 Bandwidth: **4**
 Dilution Factor: **1.0000**
 Sample Weight: **1.0000**

Chromatogram

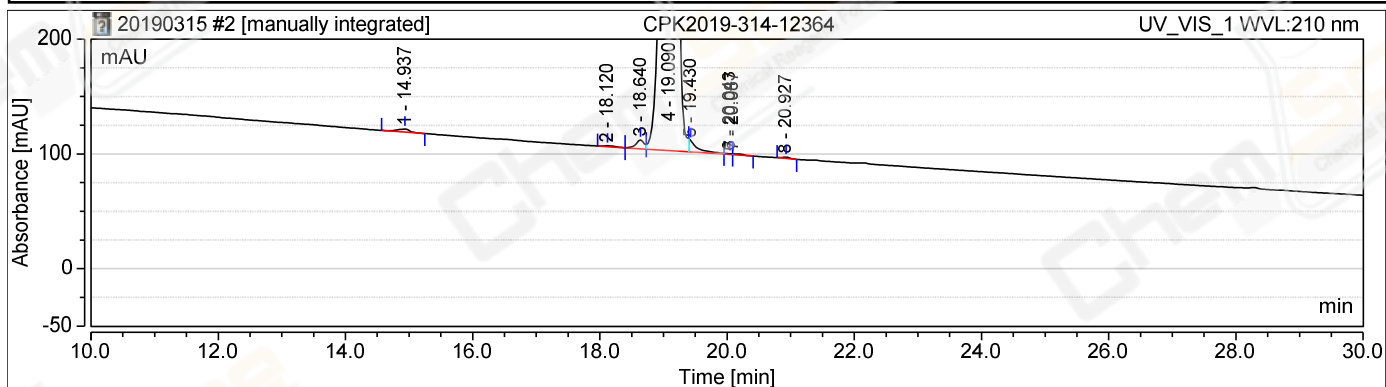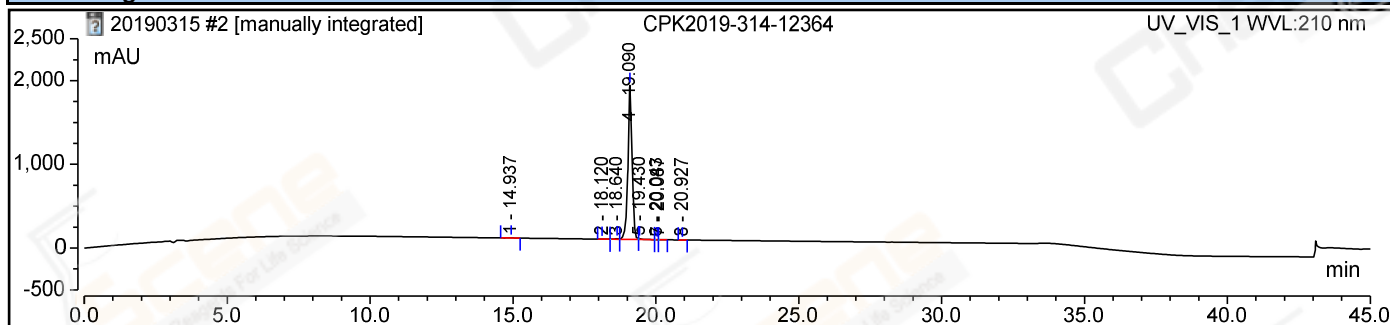

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Resolution (EP)	Match	Asymmetry (EP)	Rel.Area %
1		14.937	0.565	2.737	8.95	999	0.82	0.18
2		18.120	0.186	0.845	1.69	977	n.a.	0.06
3		18.640	1.169	7.796	1.81	1000	n.a.	0.37
4		19.090	307.964	1841.237	n.a.	1000	0.97	98.73
5		19.430	1.661	10.107	n.a.	998	n.a.	0.53
6		20.043	0.092	0.677	n.a.	999	n.a.	0.03
7		20.087	0.146	0.553	n.a.	995	n.a.	0.05
8		20.927	0.139	1.071	n.a.	995	1.06	0.04
Total:			311.922	1865.023	12.45			2.85