
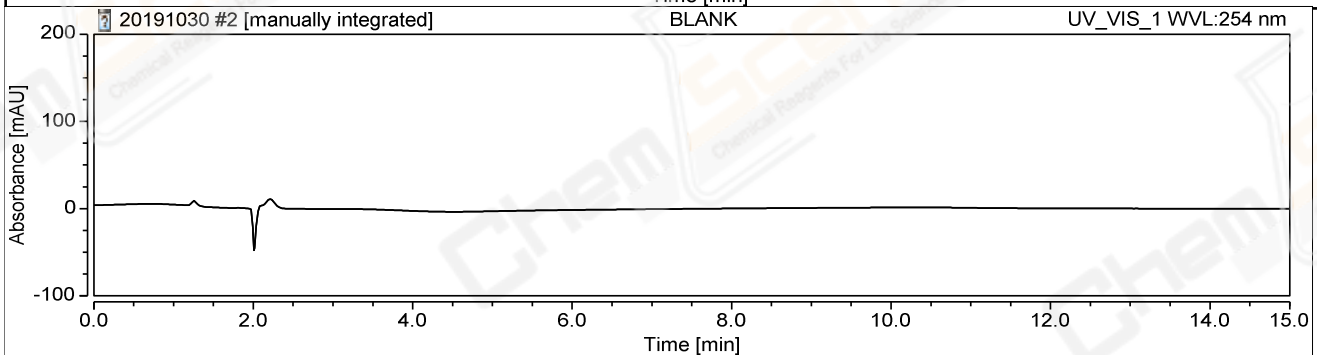


Chromatogram and Results

Injection Details

Injection Name:	BLANK	Injection Volume:	5.00
Vial Number:	GD6	Channel:	UV_VIS_1
Injection Type:	Unknown	Wavelength:	254
Calibration Level:		Users:	ly
Instrument Method:	10-80A,15MIN,254NM	Dilution Factor:	1.0000
Processing Method:	New Processing Method	Sample Weight:	1.0000
Injection Date/Time:	30/Oct/19 19:11	Run Time (min):	15.00
Catalog No:	CS-0372Batch# 12739 A-RP-327	chrom://hy261/ChromeleonLocal/Chemistry Analy/201910/20191030.seq/564.smp/UV_VIS_1.channel/UV_VIS_1.chm	

Chromatogram

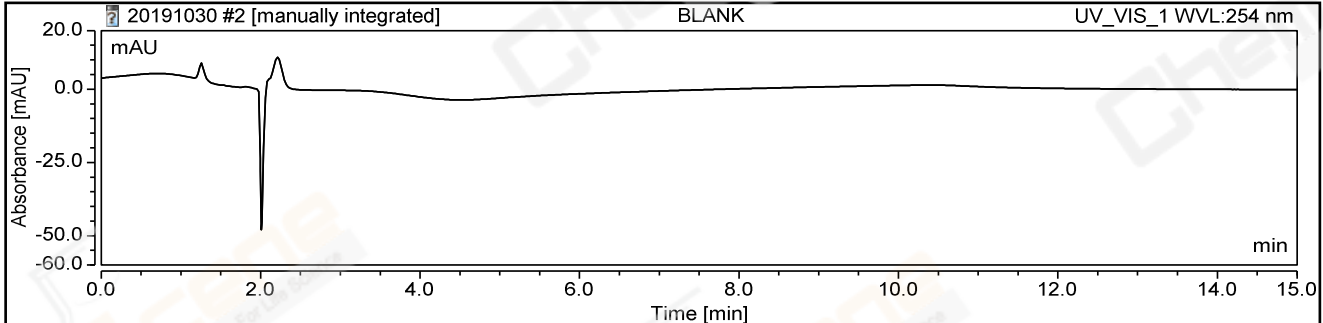

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Asymmetry (EP)	Resolution (EP)	Rel.Area %
Total:			0.000	0.000	0.00	0.00	

Chromatogram and Results

Injection Details

Injection Name: CPK2019-O29-12739	Injection Volume: 5.00
Vial Number: GD7	Channel: UV_VIS_1
Injection Type: Unknown	Wavelength: 254
Calibration Level:	Users: ly
Instrument Method: 10-80A,15MIN,254NM	Dilution Factor: 1.0000
Processing Method: New Processing Method	Sample Weight: 1.0000
Injection Date/Time: 30/Oct/19 19:27	Run Time (min): 15.00
Catalog No: CS-0372 Batch# 12739 A-RP-327	
chrom://hy261/ChromeleonLocal/Chemistry Analy/201910/20191030.seq/164.smp/UV_VIS_1.channel/UV_VIS_1.chm	

Chromatogram

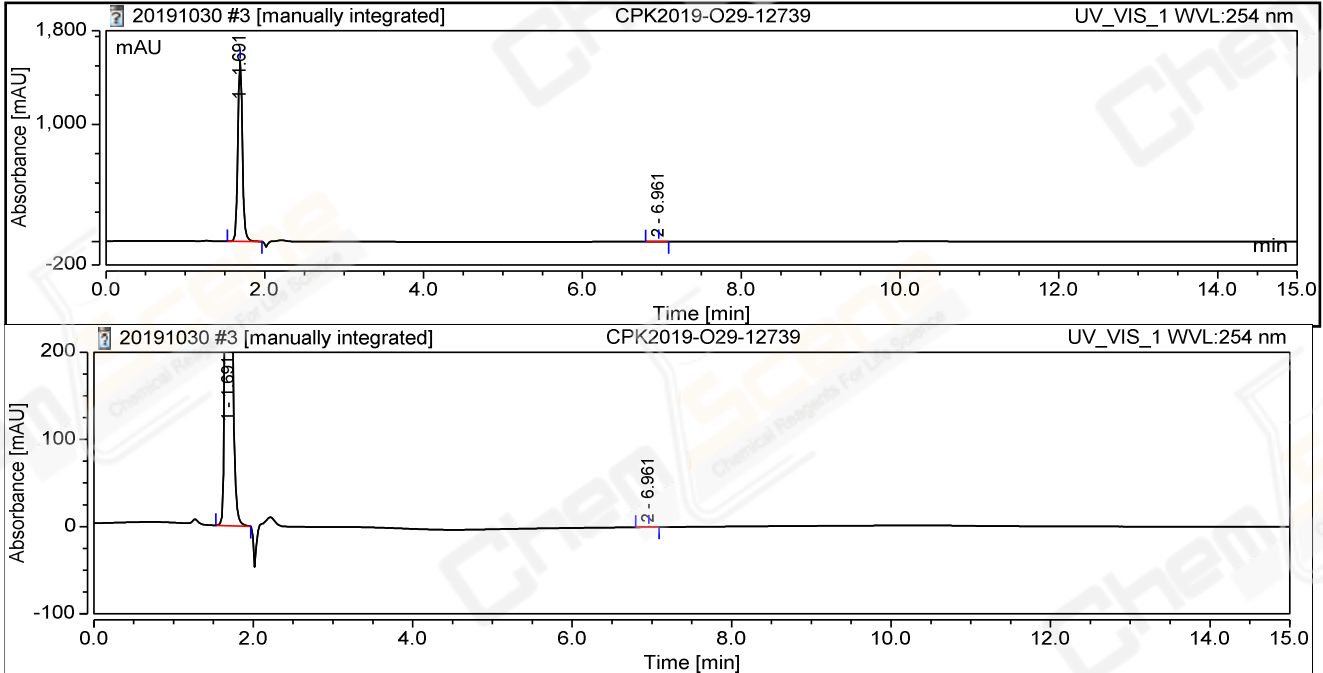

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Asymmetry (EP)	Resolution (EP)	Rel.Area %
1		1.691	105.524	1535.672	1.09	35.34	99.96
2		6.961	0.045	0.384	0.91	n.a.	0.04
Total:			105.569	1536.055	2.00	35.34	