


**2 CPK2017-816-13180****Catalog No: CS-1406 Batch#13180 A-RP-226**

Sample Name:	CPK2017-816-13180	Injection Volume:	5.0
Vial Number:	RD8	Channel:	UV_VIS_1
Sample Type:	unknown	Wavelength:	280
Control Program:	HY-303_20-H01RS10	Bandwidth:	n.a.
Quantif. Method:	default	Dilution Factor:	1.0000
Recording Time:	2017-8-17 14:14	Sample Weight:	1.0000
Run Time (min):	55.00	Sample Amount:	1.0000

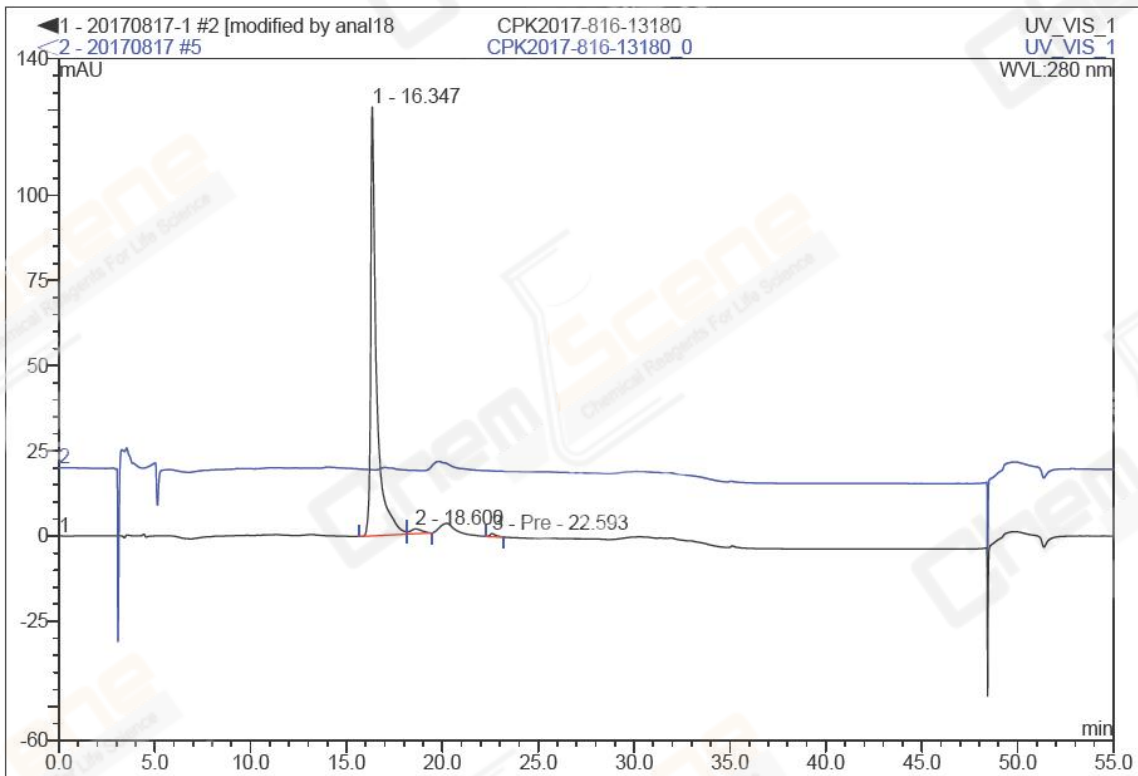

No.	Ret.Time min	Peak Name	Height mAU	Area mAU*min	Rel.Area %	Amount	Type
1	16.35	n.a.	125.784	44.592	97.21	n.a.	BM *
2	18.60	n.a.	1.395	0.971	2.12	n.a.	MB*
3	22.59	Pre	0.901	0.307	0.67	n.a.	BMB*
<b>Total:</b>			128.080	45.870	100.00	0.000	