



Chromatogram and Results

Injection Details

Injection Name:	MXY11859-033-2	Run Time (min):	30.00
Vial Number:	GD5	Users:	sy
Injection Type:	Unknown	Injection Volume:	6.00
Calibration Level:		Channel:	UV_VIS_1
Instrument Method:	HM-1113A_4-H01P06(RP-HPLC)	Wavelength:	214
Processing Method:	3D Quantitative(1)	Bandwidth:	4
CAS NO.:	2361114-15-8 A-RP-761 11/	Dilution Factor:	1.0000
Injection Date/Time:	Mar/22 14:54	Sample Weight:	1.0000

chrom://hy442/DATA2/Instrument Data/202203/20220311.seq/208.smp/UV_VIS_1.channel/UV_VIS_1.chm

Chromatogram

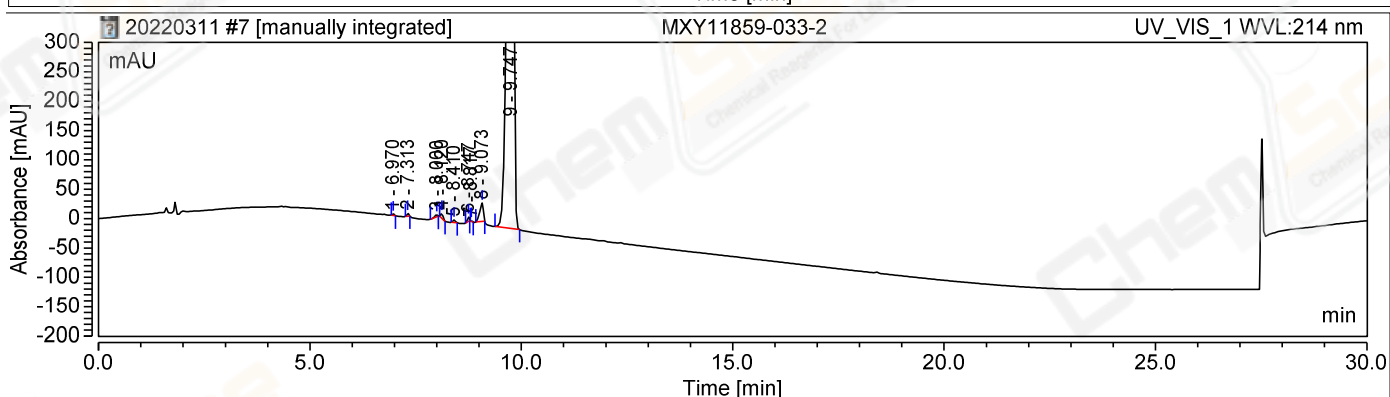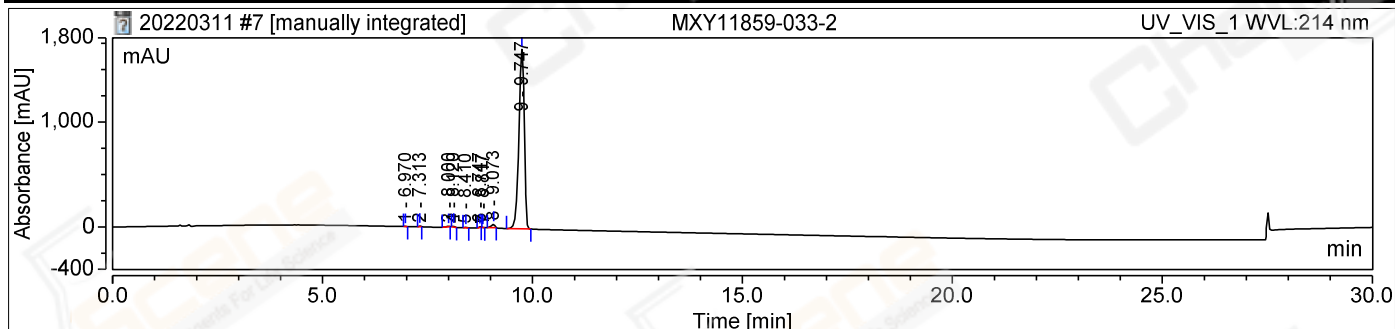

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Match	Resolution (EP)	Asymmetry (EP)	Rel.Area %
1		6.970	0.139	2.779	973	4.13	1.10	0.05
2		7.313	0.262	5.174	996	6.95	0.97	0.10
3		8.000	0.278	4.103	975	1.07	0.70	0.11
4		8.120	0.563	8.581	990	2.84	1.09	0.22
5		8.410	0.254	4.237	962	3.88	1.09	0.10
6		8.747	0.375	7.738	997	1.00	0.79	0.15
7		8.817	0.072	1.981	893	2.31	1.51	0.03
8		9.073	3.101	31.329	999	3.42	0.72	1.20
9		9.747	253.553	1708.562	937	n.a.	0.84	98.05
Total:			258.597	1774.484			25.60	8.80