


## Chromatogram and Results

### Injection Details

CAS NO.:	139652-01-0	Run Time (min):	20.00
Vial Number:	RA3	Injection Volume:	5.00
Injection Type:	Unknown	Channel:	UV_VIS_1
Calibration Level:		Wavelength:	220
Instrument Method:	HW1793	Bandwidth:	n.a.
Processing Method:	HW1793	Dilution Factor:	1.0000
Injection Date/Time:	17/8/22 12:03	Sample Weight:	1.0000

### Chromatogram

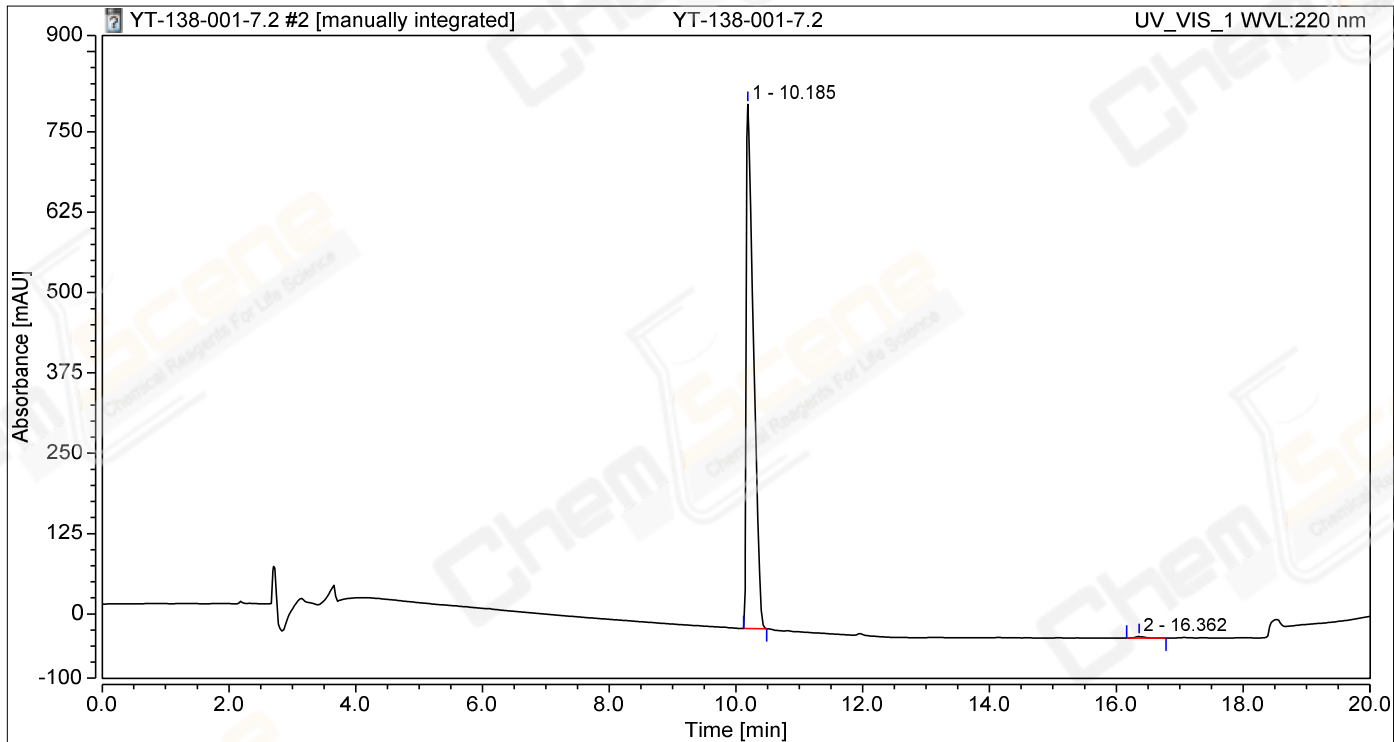

### Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount n.a.
1		10.185	107.579	815.804	99.67	99.73	n.a.
2		16.362	0.351	2.206	0.33	0.27	n.a.
<b>Total:</b>			<b>107.931</b>	<b>818.011</b>	<b>100.00</b>	<b>100.00</b>	