Data File D:\CHEM32\DATA\20160825\20160825 2016-08-25 10-31-20\004-1701.D
Sample Name: NZZ3667-01-7

==========

Acq. Operator : LCY(HPLC-09) Seq. Line : 17
Acq. Instrument : Instrument 1 Location : Vial 4
Injection Date : 8/25/2016 3:20:21 PM Inj : 1
Inj Volume : 5.000 µl
Acq. Method : D:\CHEM32\DATA\20160825\20160825 2016-08-25 10-31-20\5-50A(254NM).M
Last changed : 8/25/2016 3:29:22 PM by LCY(HPLC-09)
(modified after loading)
Analysis Method : D:\CHEM32\DATA\20160805\20160804 2016-08-05 08-42-16\10-80A(210NM).M
Last changed : 8/26/2016 12:26:32 PM by LCY(HPLC-09)
(modified after loading)
Catalog No : CS-0878 Batch#21522
A-RP-93

Additional Info : Peak(s) manually integrated

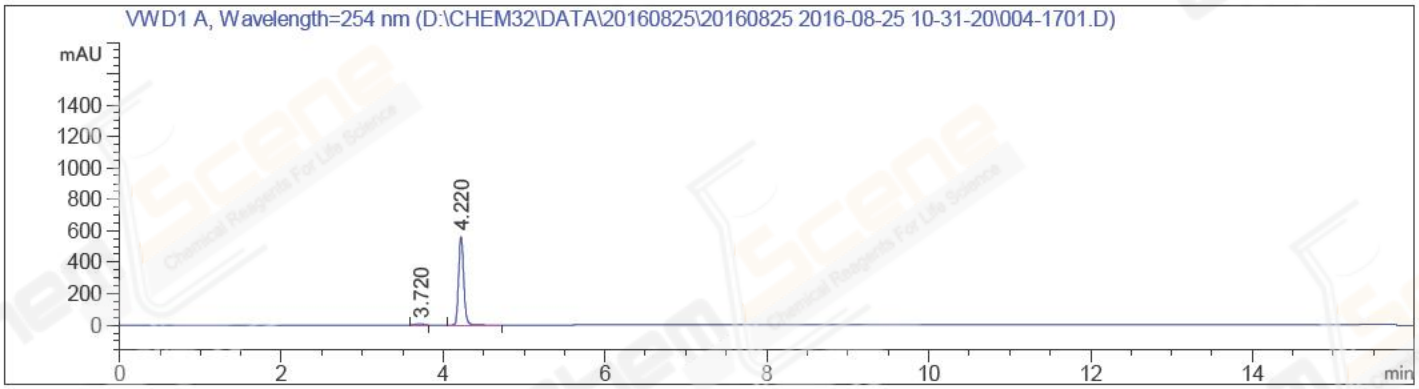

==========

Area Percent Report

==========

Sorted By : Signal
Multiplier: : 1.0000
Dilution: : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=254 nm

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	3.720	MM	0.1068	50.05621	7.81206	1.9896
2	4.220	MM	0.0727	2465.81689	565.09778	98.0104

Totals : 2515.87310 572.90983

==========

*** End of Report ***