

Sample Name: NZZ3667-013-1

```


=====
Acq. Operator   : LCY(HPLC-09)                Seq. Line :   11
Acq. Instrument : Instrument 1                 Location  : Vial 44
Injection Date  : 9/14/2016 11:40:15 AM      Inj       :    1
                                           Inj Volume: 5.000 µl

Acq. Method     : D:\CHEM32\DATA\20160914\20160914 2016-09-14 08-47-38\5-50A(254NM) .M
Last changed    : 9/14/2016 11:19:20 AM by LCY(HPLC-09)
                  (modified after loading)

Analysis Method : D:\CHEM32\METHODS\RP-HPLC\10-80A(210NM) .M
Last changed    : 9/14/2016 10:35:28 AM by LCY(HPLC-09)
                  (modified after loading)

Catalog No     : CS-0878 Batch#21694
    
```

Additional Info : Peak(s) manually integrated

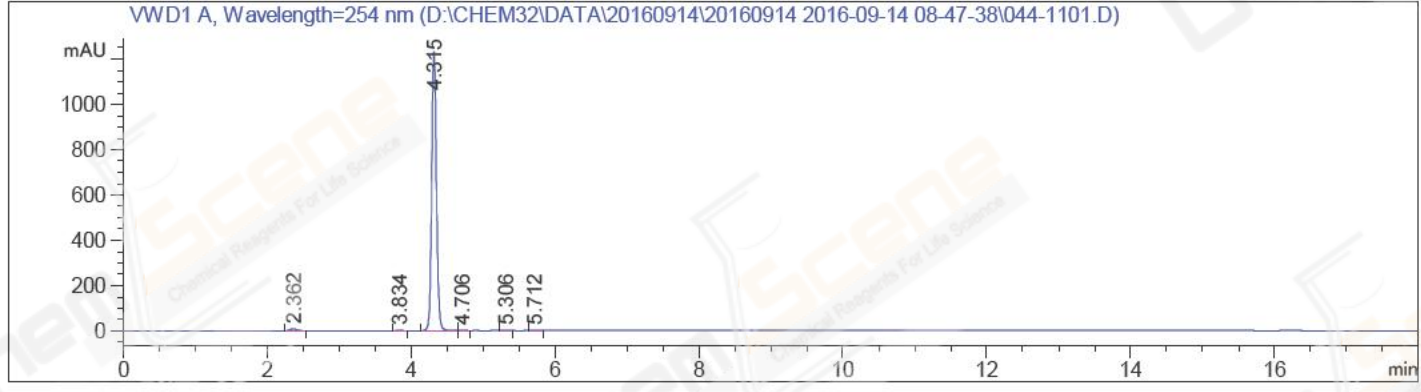

Area Percent Report

```

Sorted By      :      Signal
Multiplier:    :      1.0000
Dilution:      :      1.0000
Use Multiplier & Dilution Factor with ISTDs
    
```

Signal 1: VWD1 A, Wavelength=254 nm

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	2.362	BB	0.1031	54.53700	8.35694	0.9555
2	3.834	BB	0.0661	12.40041	2.94448	0.2173
3	4.315	MF	0.0760	5623.75049	1232.61145	98.5332
4	4.706	FM	0.0829	5.99531	1.20517	0.1050
5	5.306	BB	0.0631	6.79648	1.68241	0.1191
6	5.712	BB	0.0706	3.98728	8.84466e-1	0.0699

Totals : 5707.46697 1247.68491