


**Product Name:** NLS-StAx-h (TFA)  
**Sample name:** 21090019Final  
**Description:** Mobile phase: Buffer A: 0.1%TFA in H2O  
 Buffer B: 0.1%TFA in ACN  
 Gradient: 24-34% B in 20 min, Flow rate: 1ml/min  
 Column: Uni tary C18, 4.6\*150mm, 5um 100A  
 Instrument: Agilent HPLC 1100

**Instrument:** 1100  
**Injection date:** 2021/10/18 10:18:26  
**Last changed:** 2021/10/18 12:27:12

**Location:** 11  
**Injection:** 1 of 1  
**Injection volume:** 10.000  
**Acq. operator:** SYSTEM

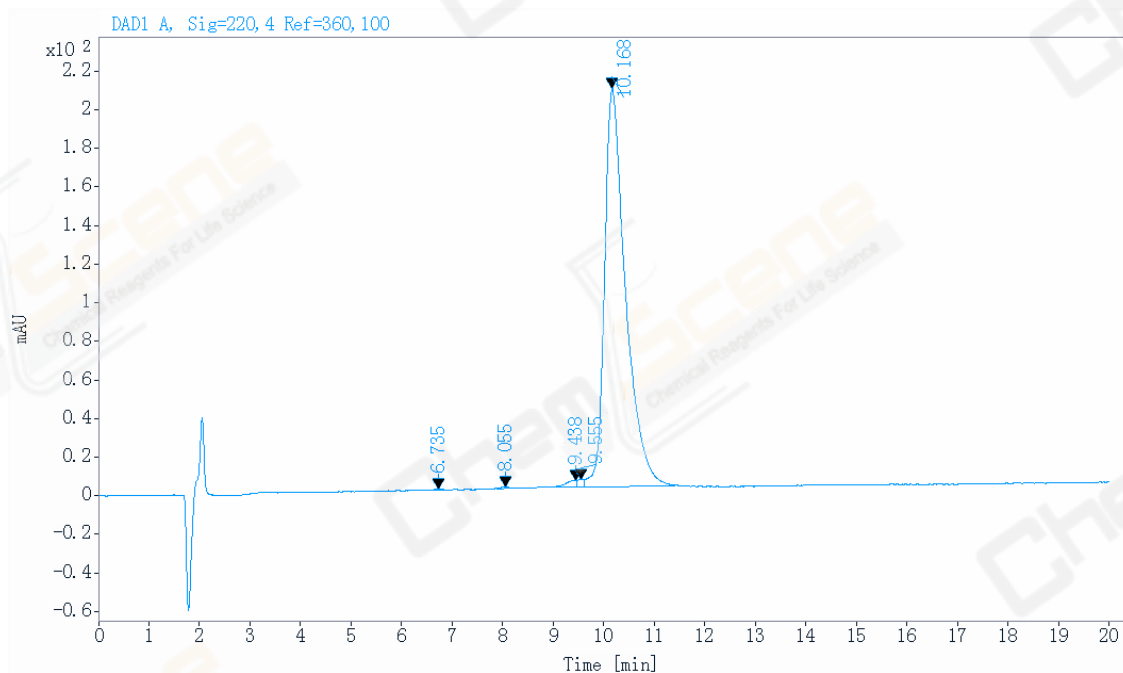

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT[mi n]	Type	Width[mi n]	Area	Height	Area% Name
6.735	BV	0.1411	8.3376	0.7535	0.1379
8.055	VV	0.1372	11.0655	1.1207	0.1830
9.438	BV	0.1684	45.3182	3.4240	0.7495
9.555	VV	0.1069	28.5411	3.5860	0.4720
10.168	VV	0.4190	5953.5122	206.1242	98.4577
Sum			6046.7746		