


SAMPLE INFORMATION

Product Name: Autocamtide 2, amide
Sample Type: Unknown
Vial: 1:E,2
Injection #: 1
Injection Volume: 5.00 ul
Run Time: 16.0 Minutes
Date Acquired: 11/17/2022 12:39:58 PM CST
Date Processed: 11/17/2022 1:04:36 PM CST

Acquired By: SFF3978
Sample Set Name: 20221117_2
Instrument Method Name: 10_90A
Processing Method: Process
Channel Name: 2998 Ch1 214nm@4.8nm
Label A-RP-1281
Column Serial Number
Processed By: SFF3978/QC

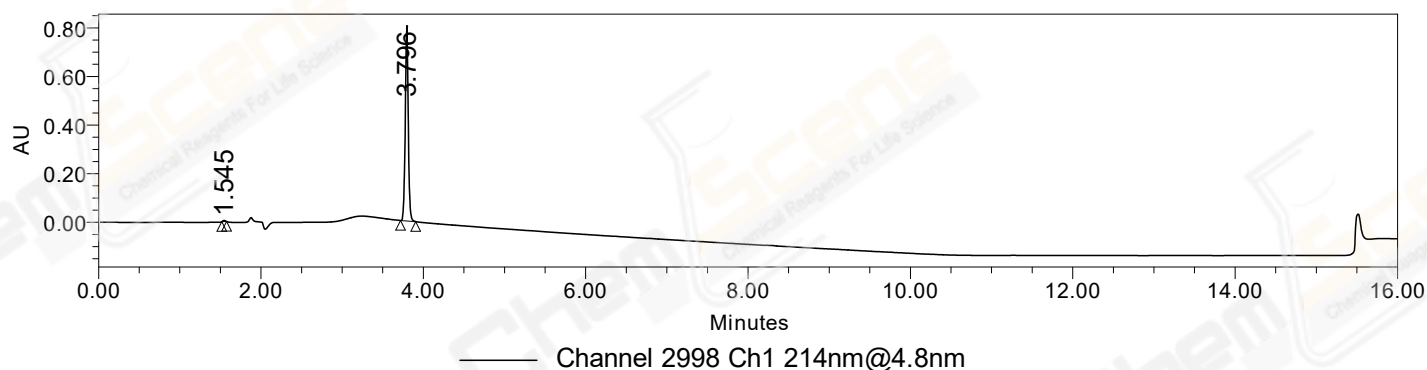

	RT	Area	Width (sec)	Height	Resolution	% Area	Name
1	1.545	10221.4298	3.500	4890.204		0.4981	
2	3.796	2041971.5115	11.200	803154.133		99.5019	