


Data file: D:\CHEM32\1\DATA\230105\603220\_23010505Final.D  
 CAS NO.: 145808-47-5  
 Description: Mobile phase: Buffer A: 0.1%TFA in H2O  
 Buffer B: 0.1%TFA in ACN  
 Gradient: 13-23% B in 20min, Flow rate: 1ml/min  
 Column: Uni tary C4, 4.6\*150mm, 5um 100A  
 Instrument: Agilent HPLC 1100  
 Instrument: 1100  
 Injection date: 2023/1/5 16:21:23  
 Last changed: 2023/1/5 16:59:46  
 Location: 57  
 Injection: 1 of 1  
 Injection volume: 10.000  
 Acq. operator: SYSTEM

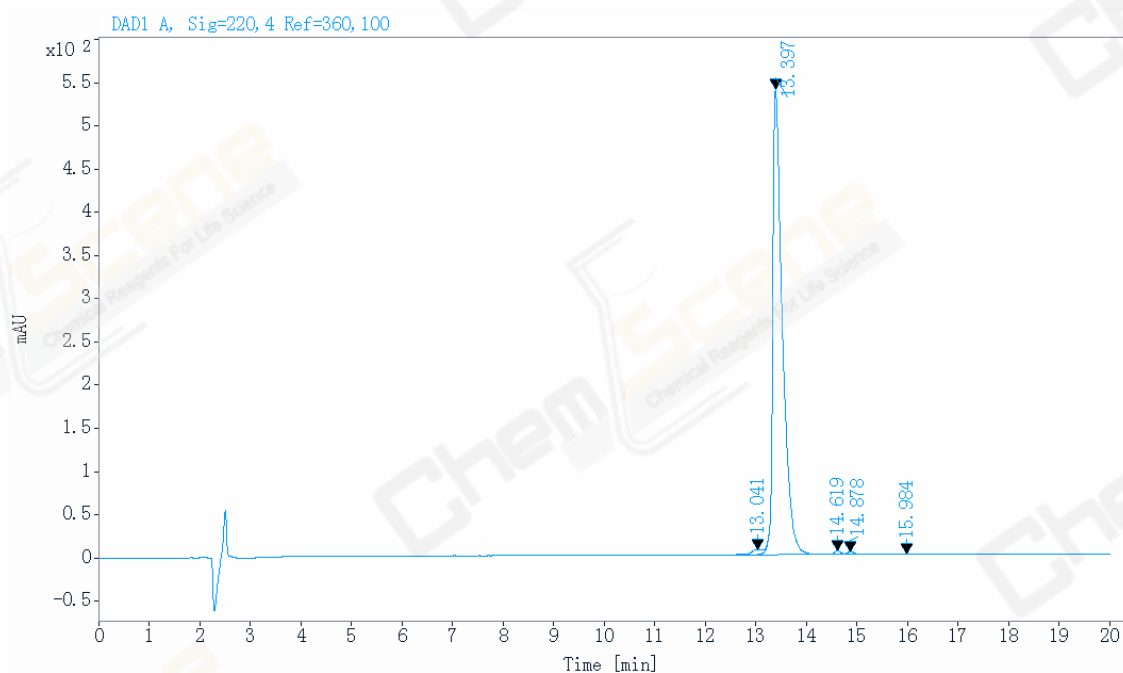

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT[mi n]	Type	Width[mi n]	Area	Height	Area%	Name
13.041	BV E	0.2487	101.9522	6.0480	1.3998	
13.397	VB R	0.1946	7109.6738	536.5068	97.6183	
14.619	BV	0.1222	33.9706	4.2081	0.4664	
14.878	VB	0.1516	33.6890	3.2867	0.4626	
15.984	VB	0.1512	3.8486	0.4187	0.0528	
	Sum		7283.1342			