

Data file: D:\CHEM32\1\DATA\230301\20230301-1 2023-03-01 12-40-46\604517
23010026Final.D

CAS NO.: 1379822-04-4


Description: Mobile phase: Buffer A: 0.1%TFA in H2O
Buffer B: 0.1%TFA in ACN
Gradient: 31-41% B in 20min, Flow rate: 1.0ml/min
Column: Unitary C18, 4.6*150mm, 5um 100A
Instrument: Agilent HPLC 1100

Instrument: 1100 Location: 46

Injection date: 2023/3/1 12:45:50 Injection: 1 of 1

Last changed: 2023/3/1 15:29:06 Injection volume: 10.000

Acq. operator: SYSTEM

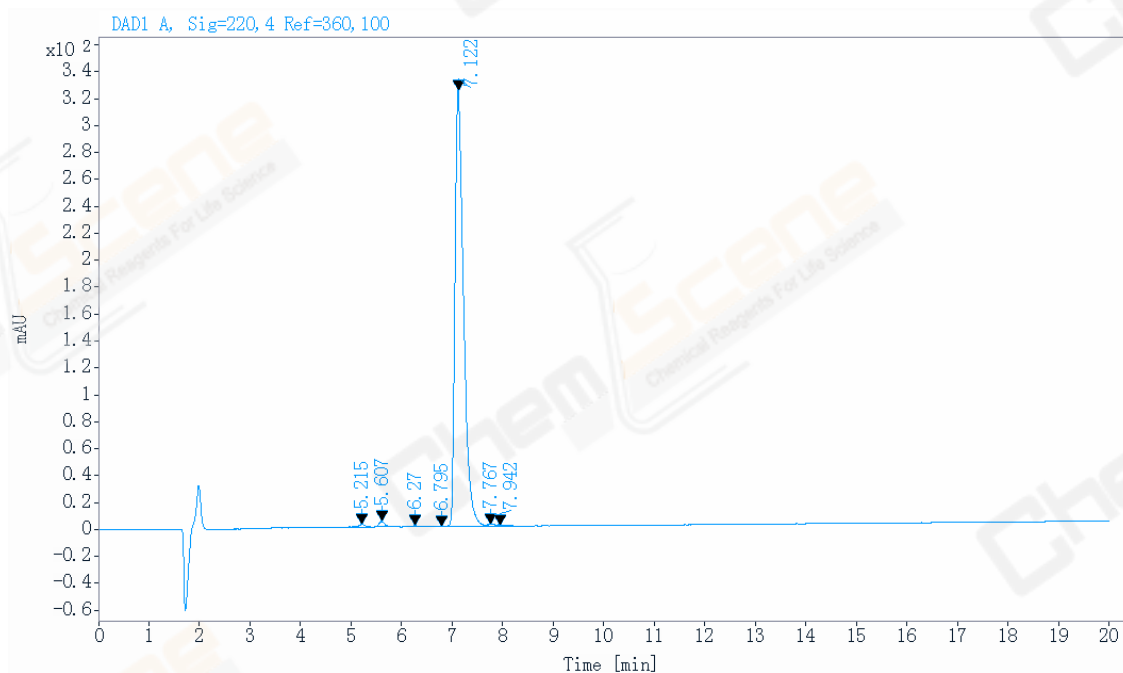

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT [min]	Type	Width [min]	Area	Height	Area%	Name
5.215	BBA	0.1311	15.8136	1.8608	0.4065	
5.607	BBA	0.1262	28.6203	3.7037	0.7357	
6.270	BBA	0.1453	5.5025	0.6597	0.1414	
6.795	BV E	0.1576	3.7198	0.3454	0.0956	
7.122	VV R	0.1805	3812.8977	325.8210	98.0084	
7.767	VV E	0.1591	12.9318	1.2666	0.3324	
7.942	VBAE	0.1684	10.8945	0.9056	0.2800	
	Sum		3890.3803			