


Data file: D:\CHEM32\1\DATA\
 CAS NO.: 452274-53-2
 Description: Mobile phase: Buffer A: 0.1%TFA in H2O
 Buffer B: 0.1%TFA in ACN
 Gradient: 22-32% B in 20min , Flow rate: 1ml/min
 Column: Uni tary C18, 4. 6*150mm, 5um 100A
 Instrument: Agilent HPLC 1100
 Instrument: 1100 Location: 43
 Injection date: 2023/6/19 15: 11: 13 Injection: 1 of 1
 Last changed: 2023/6/19 16: 03: 55 Injection volume: 10.000
 Acq. operator: SYSTEM

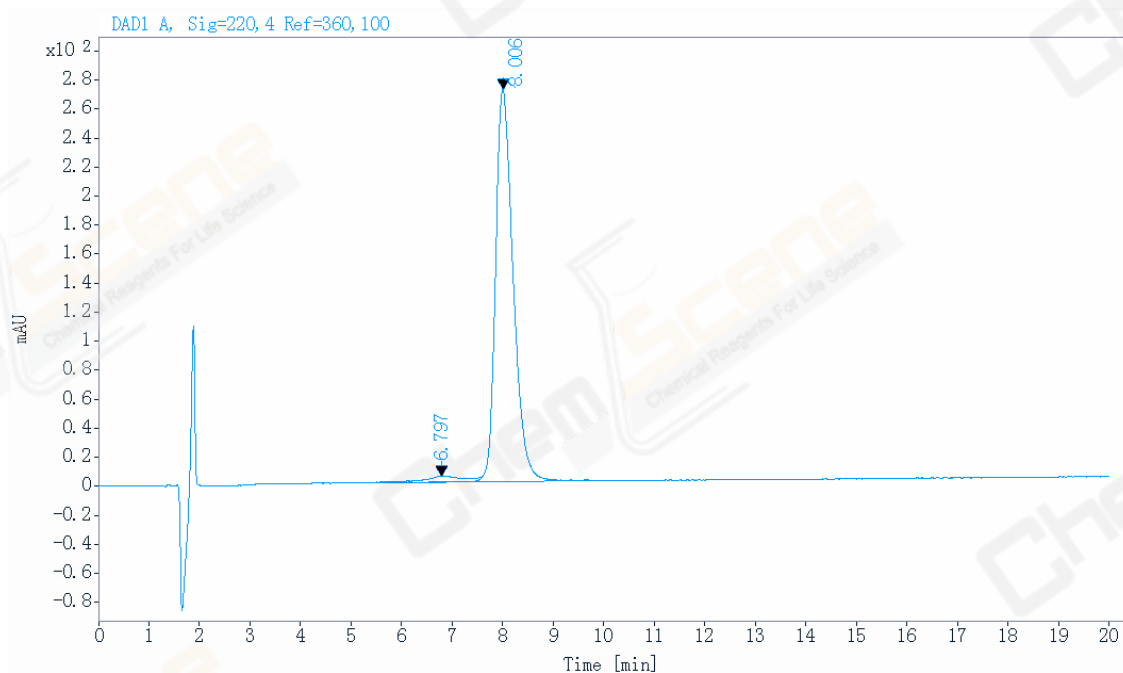

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT[mi n]	Type	Width[mi n]	Area	Height	Area% Name
6.797	VV E	0.6903	215.6844	4.3510	3.1696
8.006	VV R	0.3732	6589.0703	269.5437	96.8304
	Sum		6804.7547		