
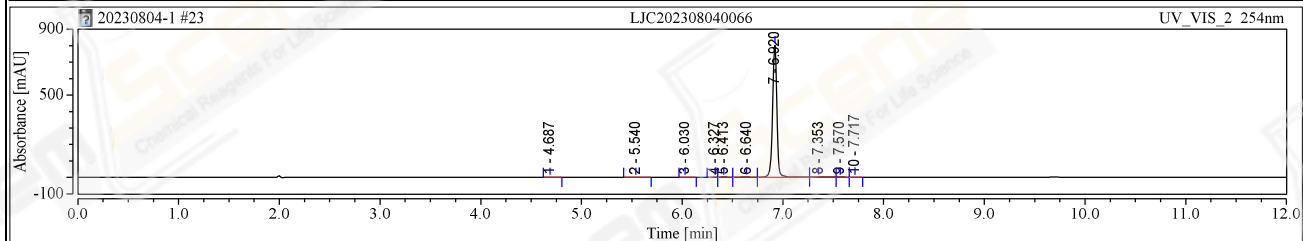


## Chromatogram and Results

Sample ID: LJC202308040066	CAS NO.: 146549-21-5
Batch No:	Channel:
Vial Number: BA7	Wavelength: 214.0
Injection Type: Unknown	Injection Volume: 5.00
Instrument: LC10410	Injection Time: 04/08/2023 17:22
Instrument Method: 10-80A-12min(LP-HPLC)	InstMeth.creation: 15/04/2022 17:33
Processing Method: LJC202308040066	Last update_time: 07/08/2023 10:41
seq.creation_operator: Azhangl	

ence/202308/Sequence/20230804-1.seq/454.smp/UV\_VIS\_1.channel/UV\_VIS\_1.chm

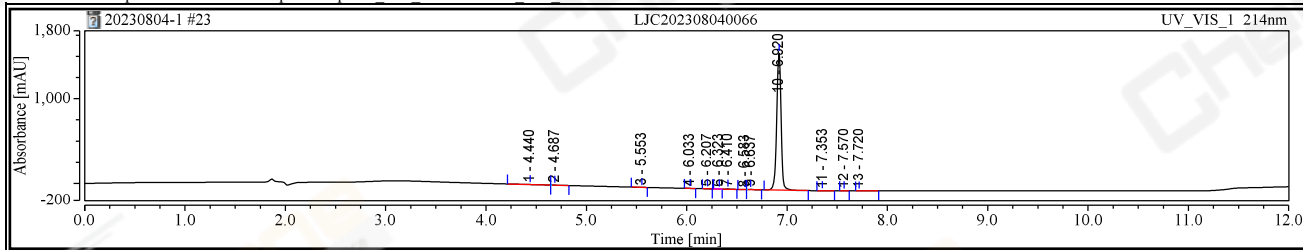

No.	Retention Time min	Area mAU*min	Height mAU	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	4.440	0.080	0.273	871	0.64	n.a.	0.100	
2	4.687	0.020	0.224	11566	5.79	n.a.	0.025	
3	5.553	0.010	0.126	31443	4.67	0.74	0.013	
4	6.033	0.019	0.391	90097	2.22	0.95	0.024	
5	6.207	0.010	0.214	107956	2.63	0.94	0.012	
6	6.323	0.009	0.208	n.a.	n.a.	n.a.	0.011	
7	6.410	0.162	2.875	104664	4.35	0.76	0.201	
8	6.583	0.030	0.772	4041393899	1.38	n.a.	0.038	
9	6.637	0.189	3.828	119605	3.72	n.a.	0.235	
10	6.920	79.872	1613.658	134356	4.85	0.94	99.225	
11	7.353	0.060	0.892	81159	2.49	1.33	0.075	
12	7.570	0.017	0.399	184360	1.51	1.03	0.021	
13	7.720	0.017	0.110	58122	n.a.	3.50	0.022	
<b>Total:</b>		<b>80.496</b>	<b>1623.969</b>		<b>34.25</b>			

No.	Retention Time min	Area mAU*min	Height mAU	Plates (USP)	Resolution (USP)	Asymmetry (USP)	Rel.Area %	Peak Name
1	4.687	0.010	0.206	69053	8.36	0.98	0.026	
2	5.540	0.015	0.162	27890	4.58	1.01	0.038	
3	6.030	0.015	0.250	88044	2.63	1.45	0.038	
4	6.327	0.014	0.236	30733	0.76	n.a.	0.035	
5	6.413	0.074	1.328	94962	2.77	n.a.	0.188	
6	6.640	0.116	1.736	109369	3.64	n.a.	0.296	
7	6.920	38.789	801.015	141454	3.54	0.94	98.742	
8	7.353	0.212	1.630	29462	1.40	n.a.	0.539	
9	7.570	0.031	0.389	48716	1.07	n.a.	0.079	
10	7.717	0.008	0.093	51590	n.a.	n.a.	0.020	
<b>Total:</b>		<b>39.283</b>	<b>807.044</b>		<b>28.76</b>			