


**14 BIZ2018-412-CXL1****Catalog No: CS-4256 Batch#29583 A-RP-281**

Sample Name:	BIZ2018-412-CXL1	Injection Volume:	5.0
Vial Number:	BA7	Channel:	UV_VIS_1
Sample Type:	unknown	Wavelength:	214
Control Program:	10-90A 214NM	Bandwidth:	n.a.
Quantif. Method:	default	Dilution Factor:	1.0000
Recording Time:	2018-4-18 17:52	Sample Weight:	1.0000
Run Time (min):	16.00	Sample Amount:	1.0000

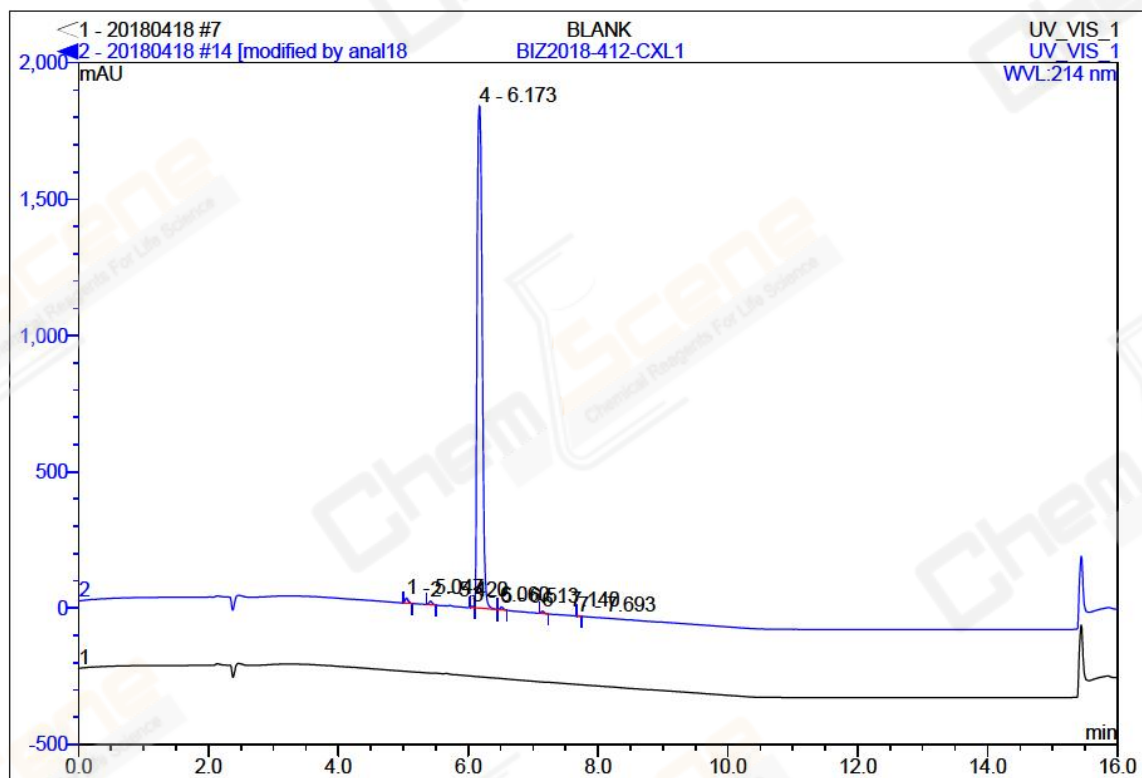

No.	Ret.Time min	Peak Name	Height mAU	Area mAU*min	Rel.Area %	Amount	Type
1	5.05	n.a.	18.020	0.971	0.58	n.a.	BMB*
2	5.42	n.a.	13.605	0.802	0.48	n.a.	BMB*
3	6.06	n.a.	5.484	0.244	0.14	n.a.	BM *
4	6.17	n.a.	1842.475	165.466	98.18	n.a.	M *
5	6.51	n.a.	10.297	0.557	0.33	n.a.	MB*
6	7.14	n.a.	8.359	0.461	0.27	n.a.	BMB*
7	7.69	n.a.	0.749	0.036	0.02	n.a.	BMB*
<b>Total:</b>			1898.990	168.537	100.00	0.000	