


Data file: C:\CHEM32\1\DATA\231214\20231214_2023-12-14_11-51-22\605950
 23110125Fianl.D
 CAS NO.: 2247635-24-9
 Description: Mobile Phase: Buffer A: 0.1% TFA in H2O
 Buffer B: 0.1% TFA in ACN
 Gradient: 35-45%B in 20min, Flow rate: 1ml/min
 Column: Unitary C18 5um 100A 4.6*150mm
 Instrument: Agilent HPLC 1100
 Instrument: 1100 Location: 94
 Injection date: 2023/12/14 11:56:23 Injection: 1 of 1
 Last changed: 2023/12/14 13:44:23 Injection volume: : 10.000

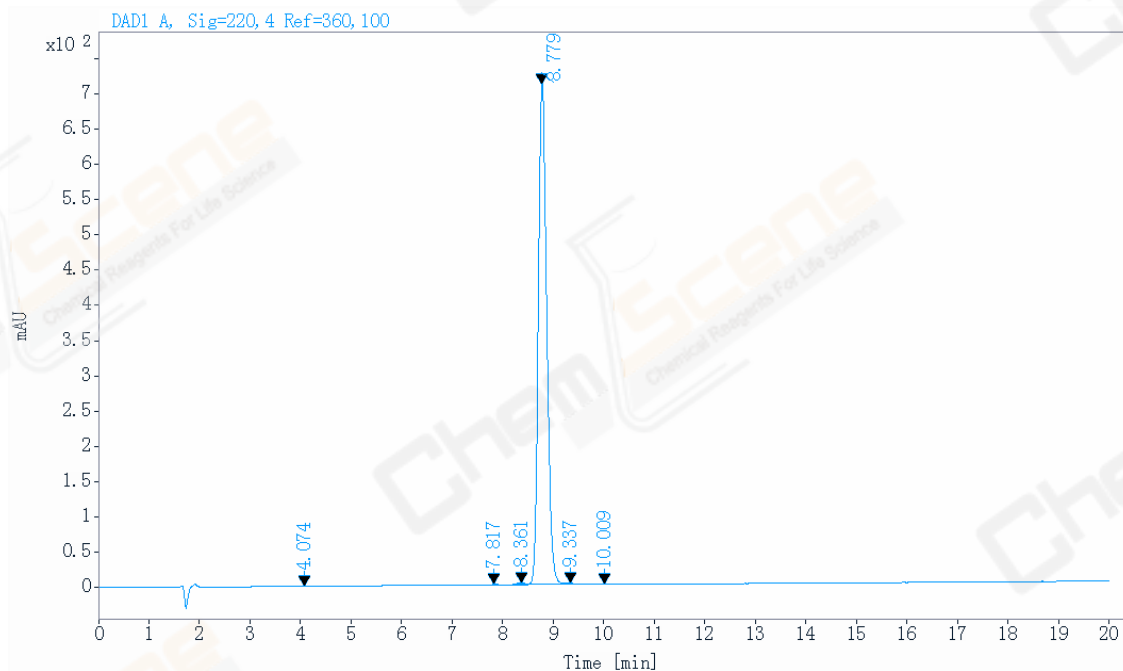

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT [min]	Type	Width [min]	Area	Height	Area%	Name
4.074	BV	0.1283	6.9235	0.8057	0.0829	
7.817	VV E	0.1314	7.3206	0.7955	0.0876	
8.361	VV E	0.1944	36.8907	2.9390	0.4416	
8.779	VF R	0.1837	8262.7080	710.3447	98.9103	
9.337	VV B	0.2077	24.3308	1.7774	0.2913	
10.009	VB	0.3898	15.5611	0.5250	0.1863	
	Sum		8353.7346			