
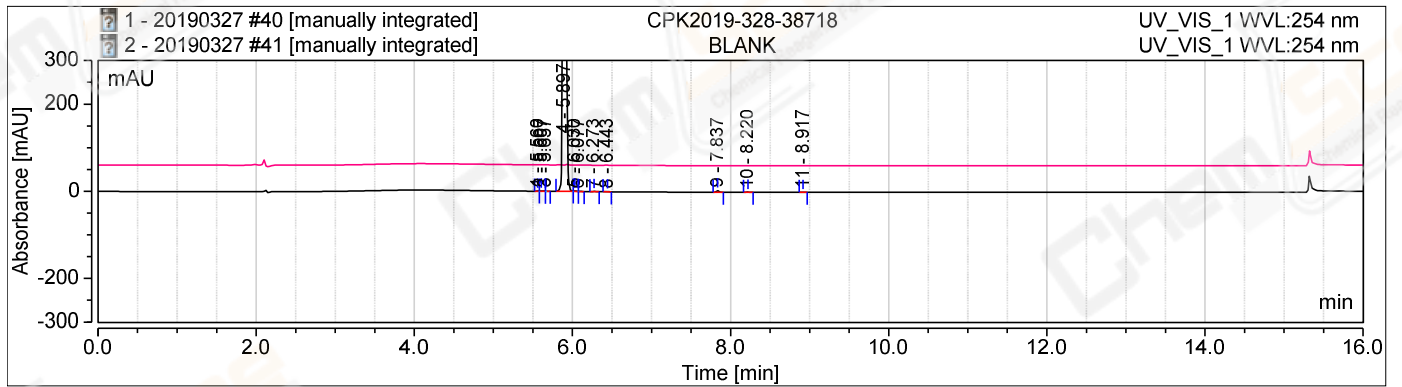


## Chromatogram and Results

Injection Details			
Injection Name:	CPK2019-328-38718	Run Time (min):	16.00
Vial Number:	BB8	Users:	zqq
Injection Type:	Unknown	Injection Volume:	1.50
Calibration Level:		Channel:	UV_VIS_1
Instrument Method:	10-90A 254NM	Wavelength:	254
Processing Method:	3D Quantitative	Bandwidth:	4
Catalog No:	CS-0033435 Batch#38718 A-RP-32	Dilution Factor:	1.0000
Injection Date/Time:	29/Mar/19 11:05	Sample Weight:	1.0000

### Chromatogram

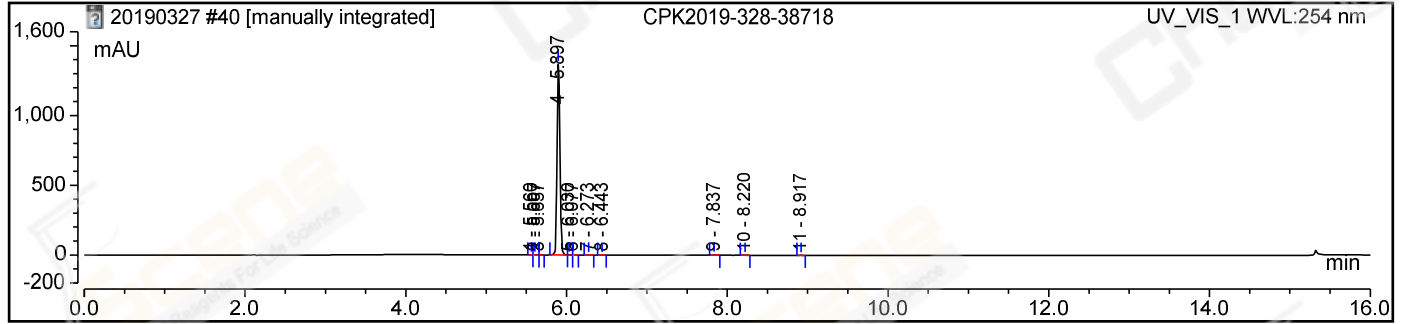

### Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Resolution (EP)	Match	Asymmetry (EP)	Rel.Area %
1		5.560	0.026	0.673	n.a.	857	n.a.	0.05
2		5.607	0.046	0.947	n.a.	657	n.a.	0.08
3		5.657	0.009	0.273	n.a.	819	n.a.	0.02
4		5.897	56.018	1367.247	n.a.	960	1.19	99.31
5		6.030	0.062	1.492	n.a.	954	n.a.	0.11
6		6.077	0.010	0.192	n.a.	667	n.a.	0.02
7		6.273	0.032	0.797	2.46	669	1.07	0.06
8		6.443	0.022	0.460	20.00	664	0.90	0.04
9		7.837	0.151	3.799	5.76	972	1.01	0.27
10		8.220	0.023	0.528	9.99	806	1.06	0.04
11		8.917	0.009	0.199	n.a.	804	0.94	0.02
Total:			56.408	1376.607	38.20			6.16