



## Chromatogram and Results

### Injection Details

<b>Injection Name:</b> BIZ2019-318-WYQ6	<b>Injection Volume:</b> 5.00
<b>Vial Number:</b> RD8	<b>Channel:</b> UV_VIS_1
<b>Injection Type:</b> Unknown	<b>Wavelength:</b> 210
<b>Calibration Level:</b>	<b>Users:</b> zqq
<b>Instrument Method:</b> 10-90A,214NM	<b>Dilution Factor:</b> 1.0000
<b>Processing Method:</b> New Processing Method	<b>Sample Weight:</b> 1.0000
<b>Injection Date/Time:</b> 19/Mar/19 02:14	<b>Run Time (min):</b> 18.00
<b>Catalog No:</b> CS-6150 Batch#39149 A-RP-328	

chrom://hy261/ChromeleonLocal/Chemistry Analy/201903/20190318.seq/515.smp/UV\_VIS\_1.channel/UV\_VIS\_1.chm

### Chromatogram

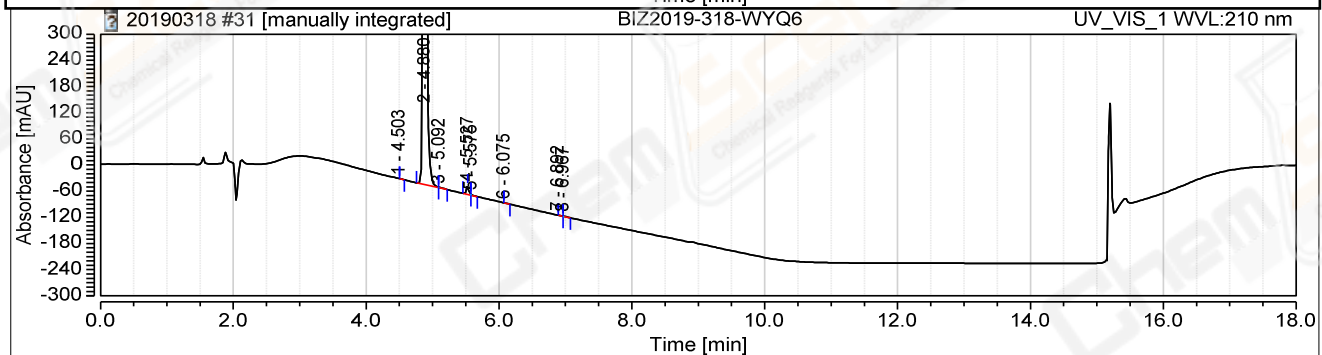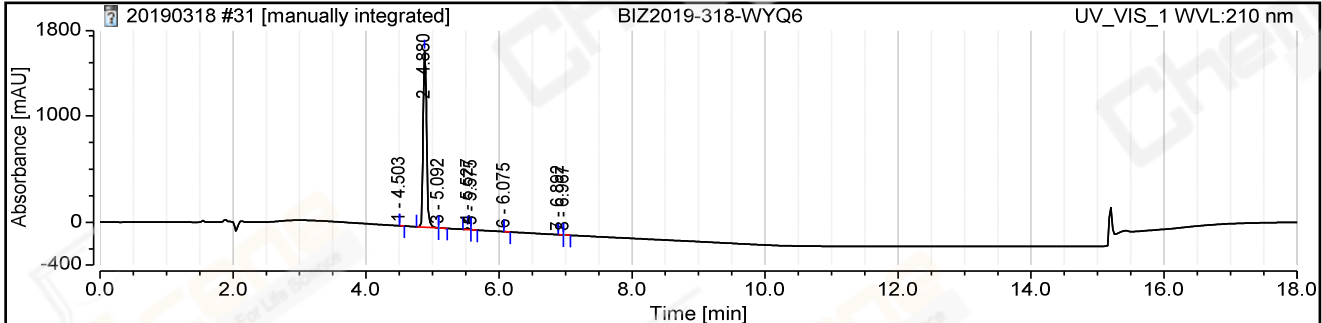

### Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Asymmetry (EP)	Resolution (EP)	Rel.Area %
1		4.503	0.016	0.000	n.a.	n.a.	0.02
2		4.880	102.631	1646.911	1.25	n.a.	98.98
3		5.092	0.100	0.862	n.a.	n.a.	0.10
4		5.527	0.804	18.875	n.a.	n.a.	0.78
5		5.575	0.065	1.759	n.a.	n.a.	0.06
6		6.075	0.014	0.000	n.a.	n.a.	0.01
7		6.892	0.011	0.000	n.a.	n.a.	0.01
8		6.967	0.047	0.152	n.a.	n.a.	0.04
<b>Total:</b>			<b>103.688</b>	<b>1668.559</b>	<b>1.25</b>	<b>0.00</b>	