



Chromatogram and Results

Injection Details

Catalog No: CS-4256 Batch#40403
Vial Number: RD4
Injection Type: Unknown
Calibration Level:
Instrument Method: 10-90A 214NM
Processing Method: 3D Quantitative
Comment: LD624_1-20190423 A-RP-328
Injection Date/Time: 24/Apr/19 11:15

Run Time (min): 16.00
Users: zqq
Injection Volume: 5.00
Channel: UV_VIS_1
Wavelength: 210
Bandwidth: 4
Dilution Factor: 1.0000
Sample Weight: 1.0000

Chromatogram

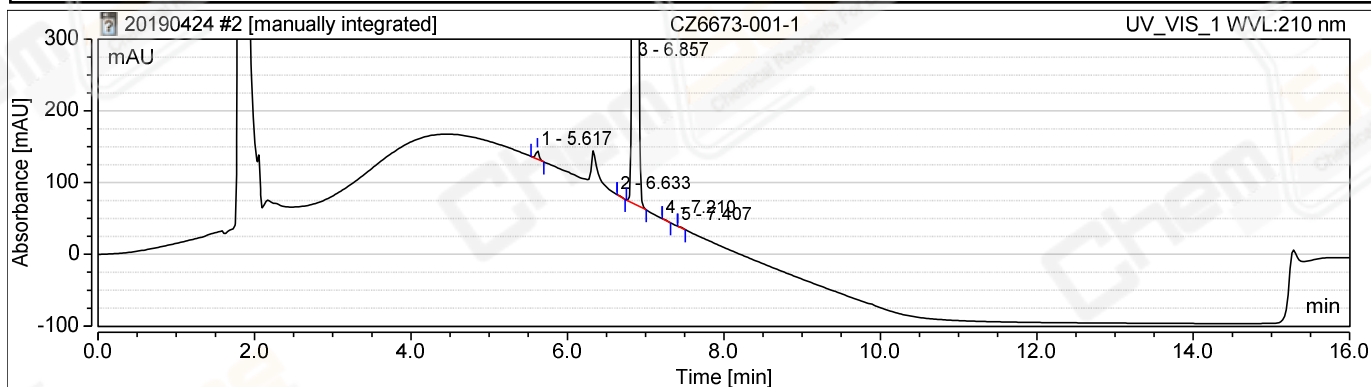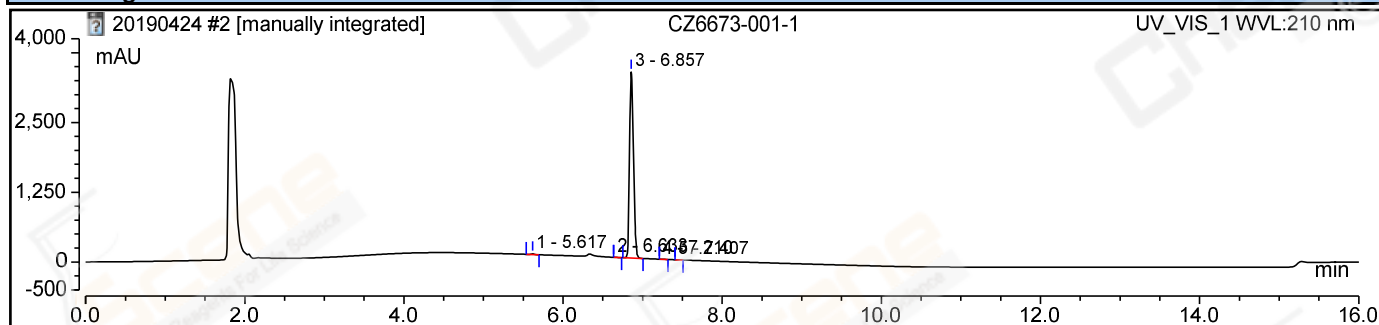

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Resolution (EP)	Match	Rel.Area %
1		5.617	0.573	12.095	n.a.	1000	0.30
2		6.633	0.045	0.000	n.a.	1000	0.02
3		6.857	188.224	3335.293	n.a.	1000	99.64
4		7.210	0.025	0.000	n.a.	1000	0.01
5		7.407	0.044	0.000	n.a.	0	0.02
Total:			188.910	3347.388	0.00	3999.66	