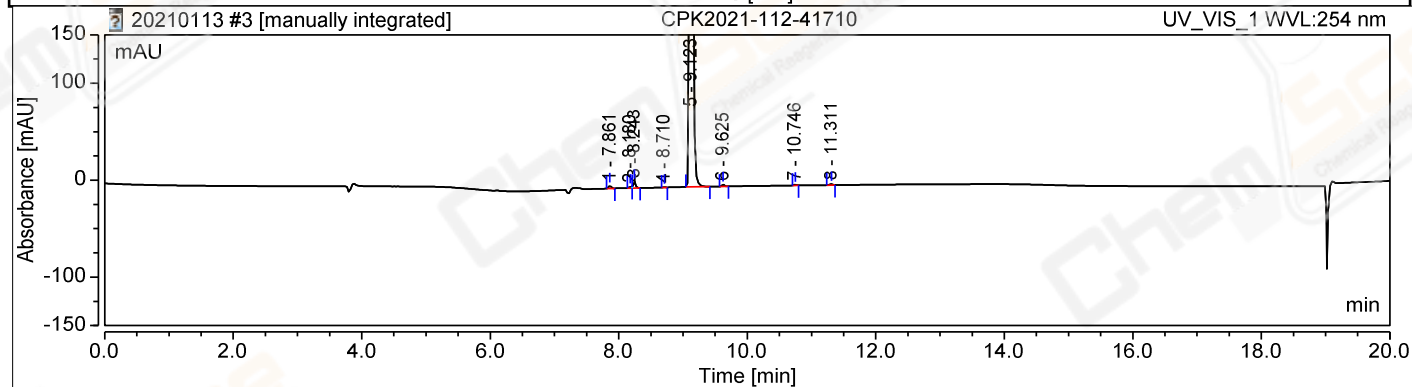
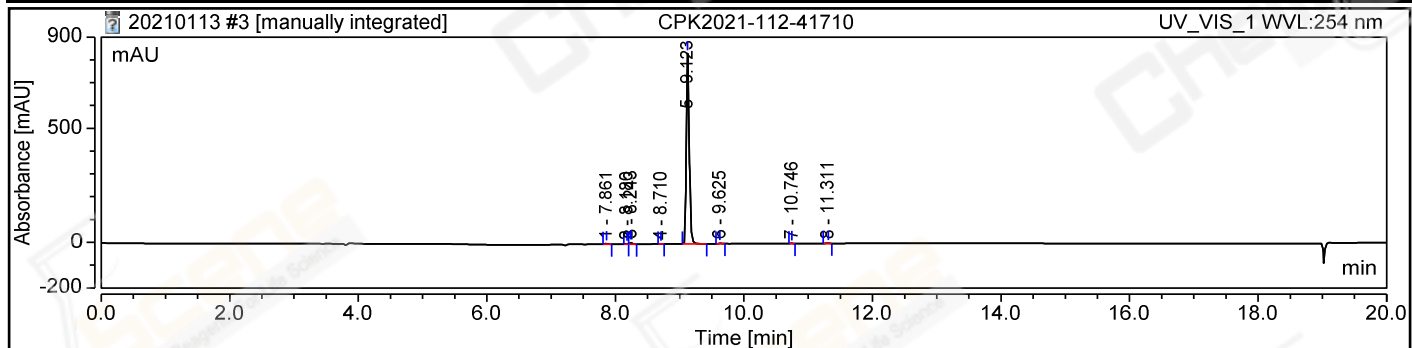


Chromatogram and Results**Injection Details**

Injection Name: CPK2021-112-41710
Vial Number: RE7
Injection Type: Unknown
Calibration Level:
Instrument Method: HY-16749-H01P01(RP-HPLC)
Processing Method: New Processing Method
Injection Date/Time: 13/Jan/21 11:57
Comment: HY-16749_20190429 A-RP-516
Injection Volume: 2.00
Channel: UV_VIS_1
Wavelength: 254
Users: jlw
Dilution Factor: 1.0000
Sample Weight: 1.0000
Run Time (min): 20.00
chrom://hy261/Themo/Instrument Data/202101/20210113.seq/732.smp/UV_VIS_1.channel/UV_VIS_1.chm

Chromatogram**Integration Results**

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Asymmetry (EP)	Plates (EP)	Rel.Area %	S/N
1		7.861	0.133	3.186	1.08	226531	0.30	0.7
2		8.180	0.069	1.661	n.a.	n.a.	0.15	0.4
3		8.243	0.289	6.566	n.a.	222613	0.65	1.4
4		8.710	0.024	0.568	1.07	262389	0.05	0.1
5		9.123	44.117	835.038	1.24	192016	98.46	180.3
6		9.625	0.090	1.997	1.31	305727	0.20	0.4
7		10.746	0.031	0.715	1.05	371090	0.07	0.2
8		11.311	0.055	1.051	0.94	295031	0.12	0.2
Total:			44.809	850.780	6.69			