


Data file: D:\CHEM32\1\DATA\230703\800024_23070301Final.D
 CAS NO.: 320367-13-3
 Description: Mobile phase: Buffer A: 0.1%TFA in H2O
 Buffer B: 0.1%TFA in ACN
 Gradient: 33-43% B in 20min, Flow rate: 1ml/min
 Column: Uni tary C18, 4.6*150mm, 5um 100A
 Instrument: Agilent HPLC 1100
 Instrument: 1100 Location: 13
 Injection date: 2023/7/3 14:22:38 Injection: 1 of 1
 Last changed: 2023/7/3 15:07:09 Injection volume: 10.000
 Acq. operator: SYSTEM

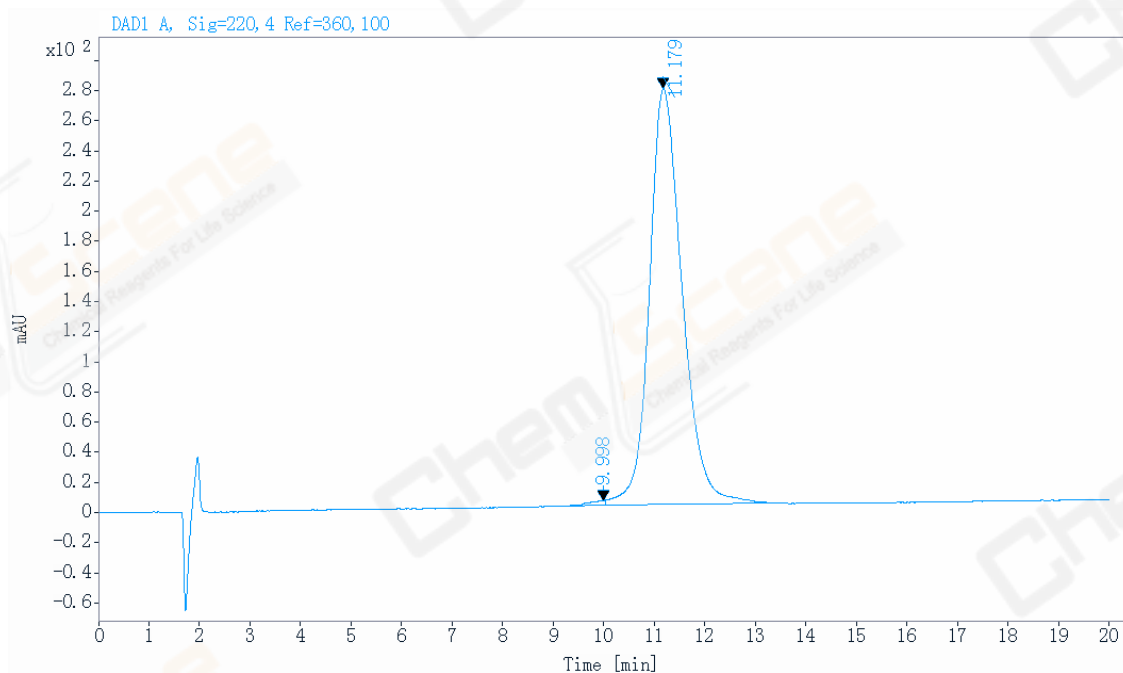

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT[mi n]	Type	Width[mi n]	Area	Height	Area% Name
9.998	MF	0.3785	79.1952	3.4872	0.6296
11.179	FM	0.7547	12498.5791	276.0182	99.3704
	Sum		12577.7743		