


**2 LJ2018-0725-0037****Catalog No: CS-M2755 Batch#43720 A-RP-281**

Sample Name:	LJ2018-0725-0037	Injection Volume:	5.0
Vial Number:	BA4	Channel:	UV_VIS_1
Sample Type:	unknown	Wavelength:	214
Control Program:	10-90A 214NM	Bandwidth:	n.a.
Quantif. Method:	default	Dilution Factor:	1.0000
Recording Time:	2018-7-26 18:48	Sample Weight:	1.0000
Run Time (min):	16.00	Sample Amount:	1.0000

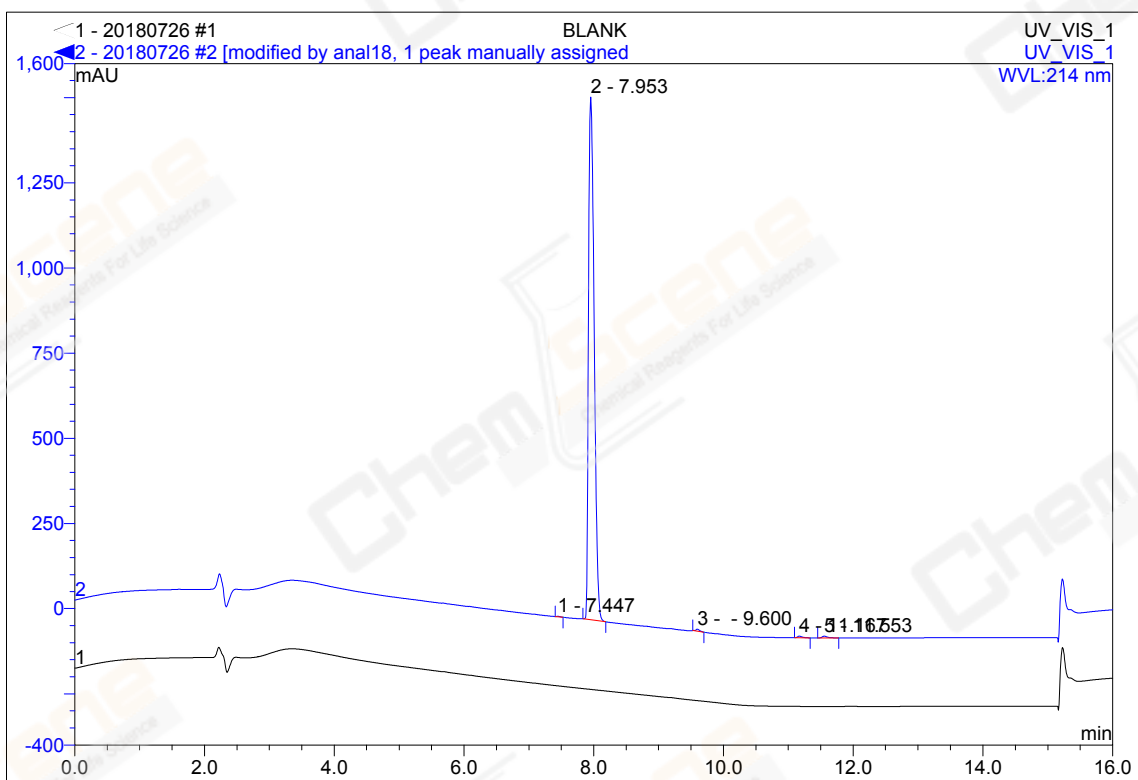

No.	Ret.Time min	Peak Name	Height mAU	Area mAU*min	Rel.Area %	Amount	Type
1	7.45	n.a.	1.443	0.090	0.06	n.a.	BMB*
2	7.95	n.a.	1534.211	155.417	99.16	n.a.	BMB*
3	9.60	n.a.	6.306	0.416	0.27	n.a.	BMB*^
4	11.17	n.a.	4.663	0.374	0.24	n.a.	BMB
5	11.55	n.a.	5.241	0.436	0.28	n.a.	BMB
<b>Total:</b>			1551.863	156.734	100.00	0.000	