
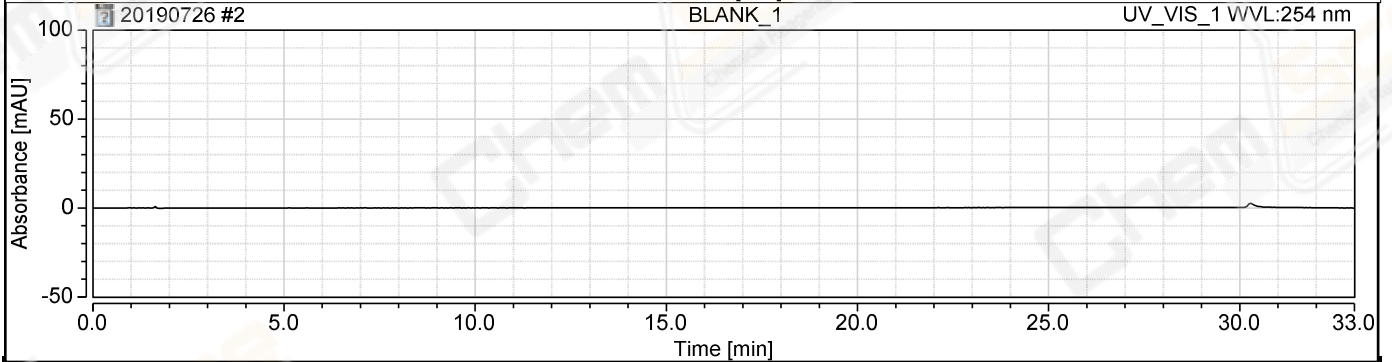


Chromatogram and Results

Injection Details

Injection Name:	BLANK_1	Run Time (min):	33.00
Vial Number:	BA1	Injection Volume:	5.00
Comment:	BLANK A-RP-422	Channel:	UV_VIS_1
Calibration Level:		Wavelength:	254
Instrument Method:	HM-149_TM-H01RS02(RP-HPLC),BD	Bandwidth:	4
COMMENT:	BLANK_1	Dilution Factor:	1.0000
Injection Date/Time:	26/Jul/19 10:20	Sample Weight:	1.0000

Chromatogram

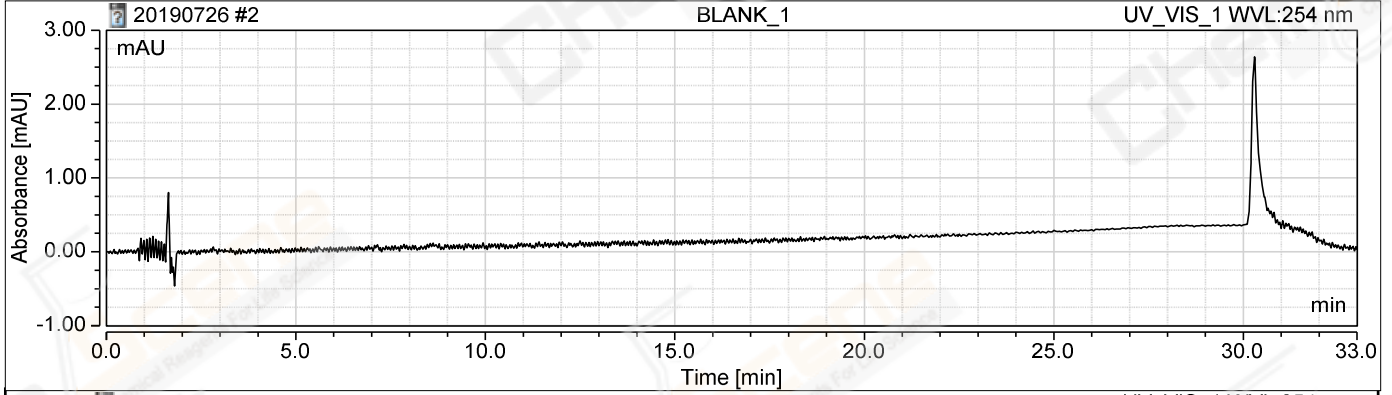

Integration Results



No.	Peak Name	Retention Time min	Area mAU*s	Height mAU	Relative Area %	S/N	Resolution (EP)
Total:			0.000	0.000	0.00	0.00	

Chromatogram and Results

Injection Details

Injection Name: CKK6869-049-9P	Run Time (min): 33.00
Vial Number: GA1	Injection Volume: 5.00
Injection Type: Unknown	Channel: UV_VIS_1
Comment: HM-149_TM-20190722 A-RP-422	Wavelength: 254
Instrument Method: HM-149_TM-H01RS02(RP-HPLC),BD	Bandwidth: 4
Processing Method: 3D Quantitative	Dilution Factor: 1.0000
Injection Date/Time: 26/Jul/19 10:55	Acq Operator: LQ

Chromatogram

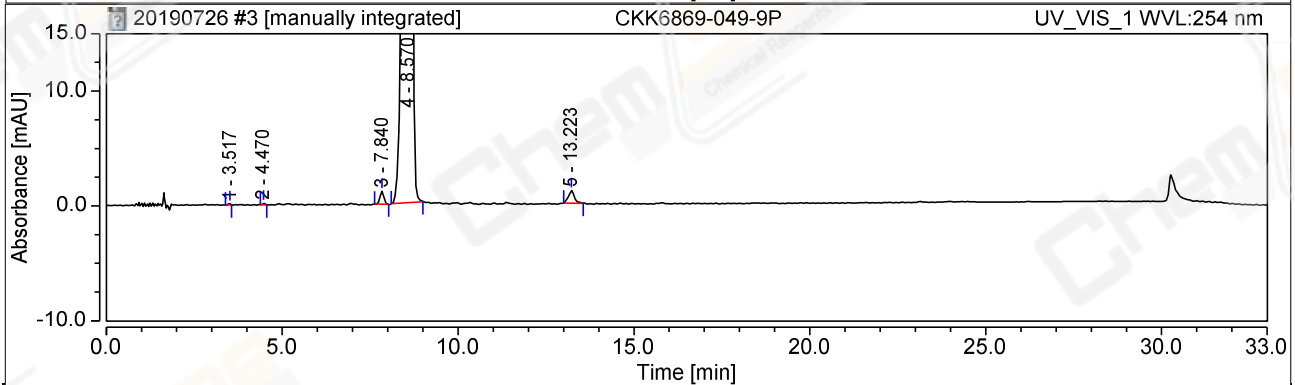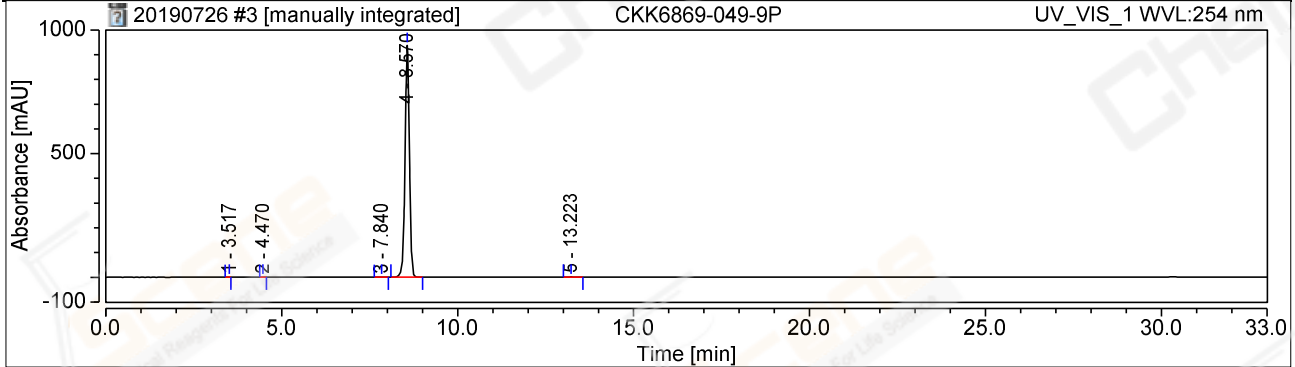

Integration Results

No.	Peak Name	Retention Time min	Area mAU*s	Height mAU	Relative Area %	Resolution	Plates	Asymmetry
1		3.517	0.532	0.123	0.01	7.91	10271	0.75
2		4.470	0.661	0.153	0.01	22.66	30569	1.54
3		7.840	8.791	1.131	0.11	3.47	25832	0.94
4		8.570	8175.920	937.645	99.72	18.06	23049	0.95
5		13.223	12.940	1.095	0.16	n.a.	33373	1.19
Total:			8198.844	940.148	100.00		123094.00	