


6 WGY7176-003-1			
Catalog No: CS-4869 Batch#47129 A-RP-341 JLW			
Sample Name:	WGY7176-003-1	Injection Volume:	5.0
Vial Number:	BA5	Channel:	UV_VIS_1
Sample Type:	unknown	Wavelength:	215
Control Program:	HY_14958A-H01P05(RP-HPLC)	Bandwidth:	n.a.
Quantif. Method:	default	Dilution Factor:	1.0000
Recording Time:	2019-10-15 14:13	Sample Weight:	1.0000
Run Time (min):	25.00	Sample Amount:	1.0000

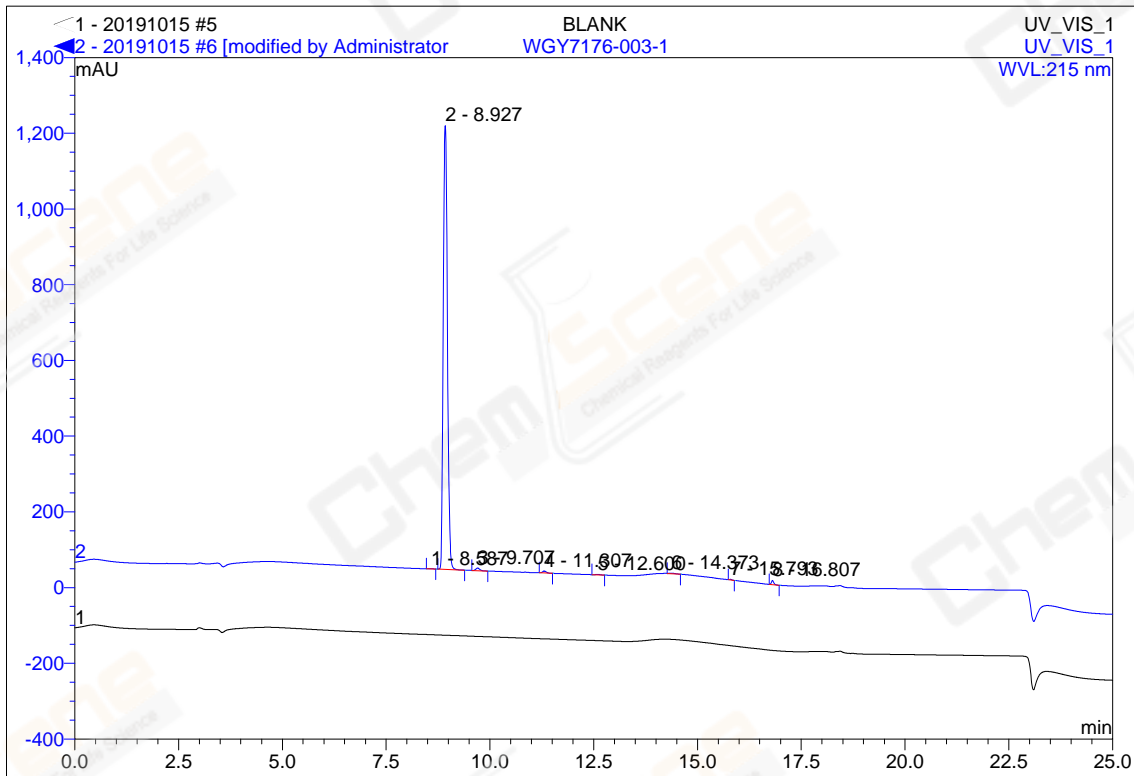

No.	Ret.Time min	Peak Name	Height mAU	Area mAU*min	Rel.Area %	Amount	Type
1	8.59	n.a.	0.856	0.077	0.05	n.a.	BMB*
2	8.93	n.a.	1172.101	139.102	98.24	n.a.	BMB*
3	9.71	n.a.	7.078	0.740	0.52	n.a.	BMB*
4	11.31	n.a.	5.149	0.498	0.35	n.a.	BMB*
5	12.60	n.a.	1.329	0.147	0.10	n.a.	BMB
6	14.37	n.a.	1.193	0.189	0.13	n.a.	BMB*
7	15.79	n.a.	1.340	0.089	0.06	n.a.	BMB
8	16.81	n.a.	11.318	0.746	0.53	n.a.	BMB
Total:			1200.364	141.587	100.00	0.000	