


<b>59 BIZ2019-N11-CXL3</b>			
<b>Catalog No: CS-1285 Batch#51799 A-RP-243 JLW</b>			
Sample Name:	<b>BIZ2019-N11-CXL3</b>	Injection Volume:	<b>5.0</b>
Vial Number:	<b>BC1</b>	Channel:	<b>UV_VIS_1</b>
Sample Type:	<b>unknown</b>	Wavelength:	<b>214</b>
Control Program:	<b>10-90A 214NM</b>	Bandwidth:	<b>n.a.</b>
Quantif. Method:	<b>default</b>	Dilution Factor:	<b>1.0000</b>
Recording Time:	<b>2019-11-13 3:40</b>	Sample Weight:	<b>1.0000</b>
Run Time (min):	<b>16.00</b>	Sample Amount:	<b>1.0000</b>

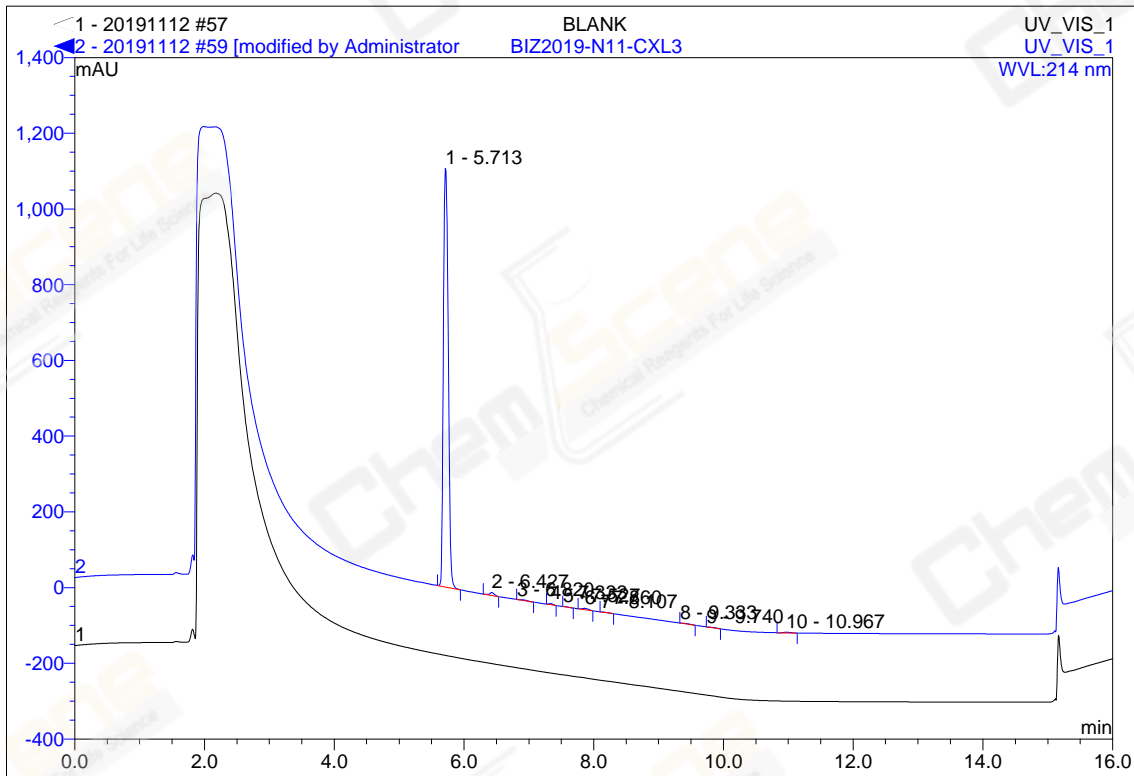

No.	Ret.Time min	Peak Name	Height mAU	Area mAU*min	Rel.Area %	Amount	Type
1	5.71	n.a.	1105.915	95.411	98.02	n.a.	MB*
2	6.43	n.a.	7.792	0.614	0.63	n.a.	BMB*
3	6.82	n.a.	0.005	0.170	0.18	n.a.	BMB*
4	7.33	n.a.	3.014	0.206	0.21	n.a.	BMB*
5	7.53	n.a.	0.065	0.051	0.05	n.a.	BMB*
6	7.86	n.a.	3.586	0.399	0.41	n.a.	BMB*
7	8.11	n.a.	0.034	0.064	0.07	n.a.	BMB*
8	9.33	n.a.	0.021	0.132	0.14	n.a.	BMB*
9	9.74	n.a.	0.016	0.095	0.10	n.a.	BMB*
10	10.97	n.a.	1.597	0.198	0.20	n.a.	BMB
<b>Total:</b>			1122.045	97.340	100.00	0.000	