


13 BIZ2019-D30-SCH2**Catalog No: CS-0008288 Batch#58493 A-RP-243 JLW**

Sample Name:	BIZ2019-D30-SCH2	Injection Volume:	2.0
Vial Number:	RD8	Channel:	UV_VIS_1
Sample Type:	unknown	Wavelength:	214
Control Program:	10-90A 214NM	Bandwidth:	n.a.
Quantif. Method:	default	Dilution Factor:	1.0000
Recording Time:	2020-1-2 18:20	Sample Weight:	1.0000
Run Time (min):	16.00	Sample Amount:	1.0000

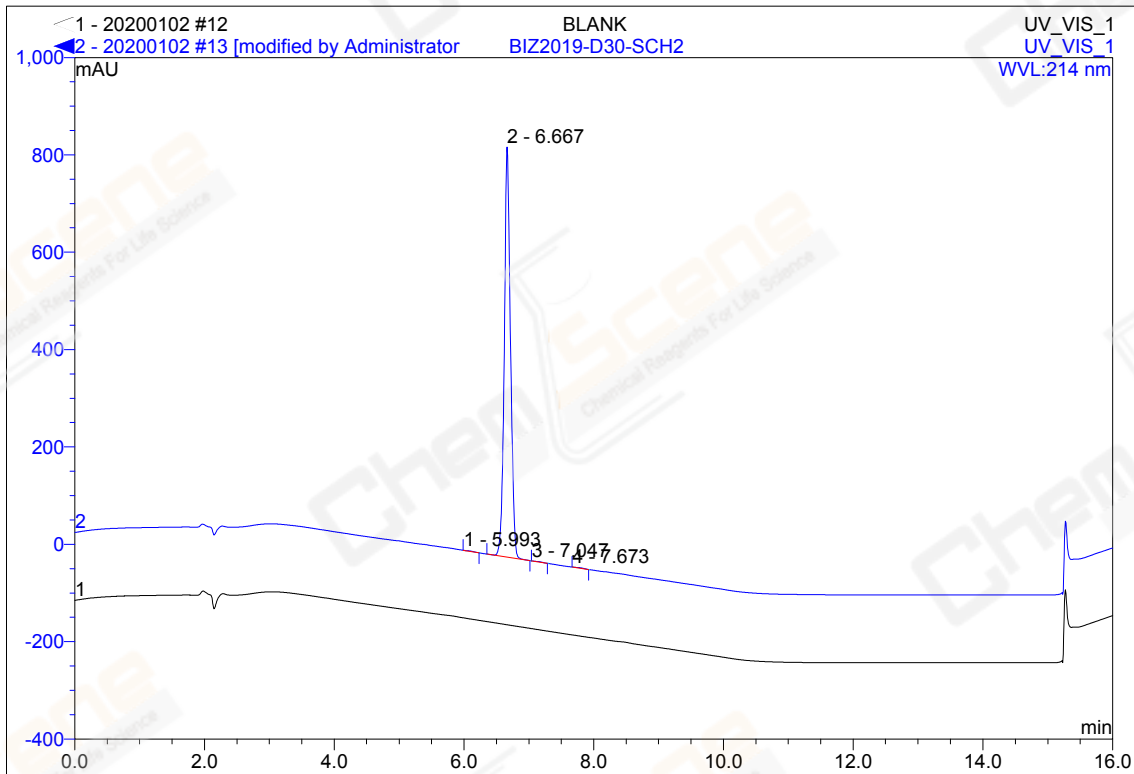

No.	Ret.Time min	Peak Name	Height mAU	Area mAU*min	Rel.Area %	Amount	Type
1	5.99	n.a.	0.007	0.089	0.09	n.a.	BMB*
2	6.67	n.a.	842.310	93.213	99.69	n.a.	BMB
3	7.05	n.a.	0.022	0.080	0.09	n.a.	BMB*
4	7.67	n.a.	0.051	0.118	0.13	n.a.	BMB*
Total:			842.389	93.500	100.00	0.000	