


CAS NO. : 65147-06-0
Description: Mobile Phase: Buffer A: 0.1% TFA in H₂O
 Buffer B: 0.1% TFA in ACN
 Gradient: 30-40%B in 20min, Flow rate: 1.0ml/min
 Column: Unitary C18 5um 100A 4.6*150mm
 Instrument: Agilent HPLC 1100
Instrument: 1100
Location: 21
Injection date: 2024/11/11 9:35:52
Injection: 1 of 1
Last changed: 2024/11/11 10:01:59
Injection volume: 5.000
Acq. operator:

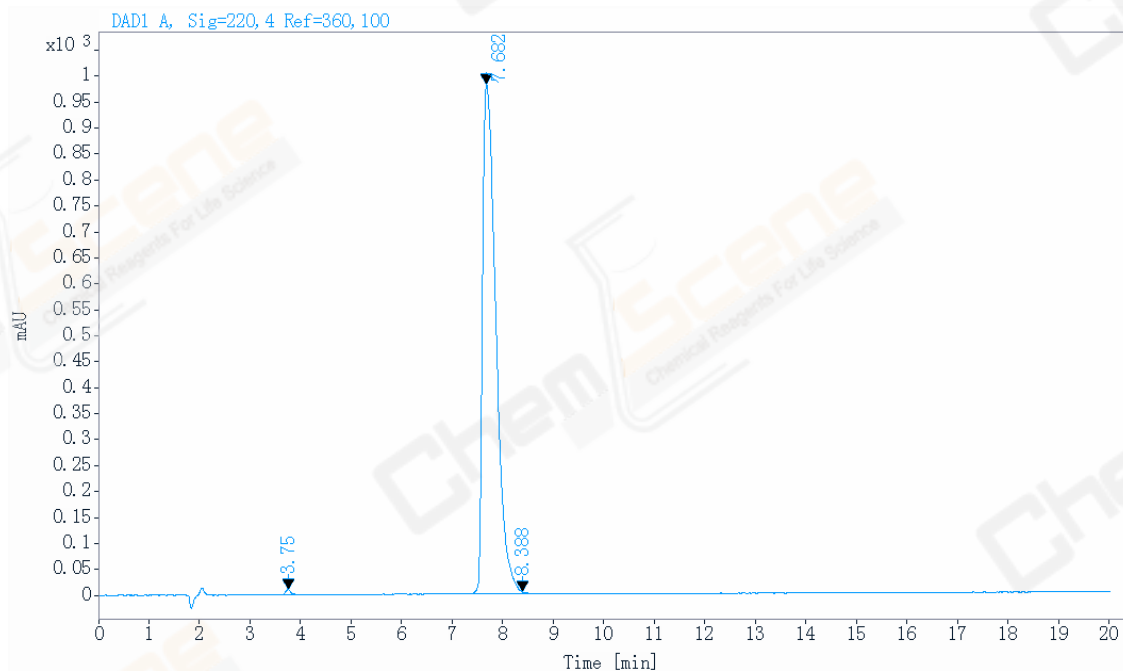

Signal : DAD1 A, Sig=220, 4 Ref=360, 100

RT [min]	Type	Width [min]	Area	Height	Area%	Name
3.750	BB	0.1092	71.1692	9.9743	0.3921	
7.682	MF	0.3065	18063.2266	982.0815	99.5092	
8.388	FM	0.0811	17.9221	3.6838	0.0987	
	Sum		18152.3178			