


27 LJ2001160040**Catalog No: CS-W013226 Batch#Ld0119036 A-RP-520 JLW**

Sample Name:	LJ2001160040	Injection Volume:	2.0
Vial Number:	BB6	Channel:	UV_VIS_1
Sample Type:	unknown	Wavelength:	214
Control Program:	10-90A 214NM	Bandwidth:	n.a.
Quantif. Method:	default	Dilution Factor:	1.0000
Recording Time:	2020-1-19 20:19	Sample Weight:	1.0000
Run Time (min):	16.00	Sample Amount:	1.0000

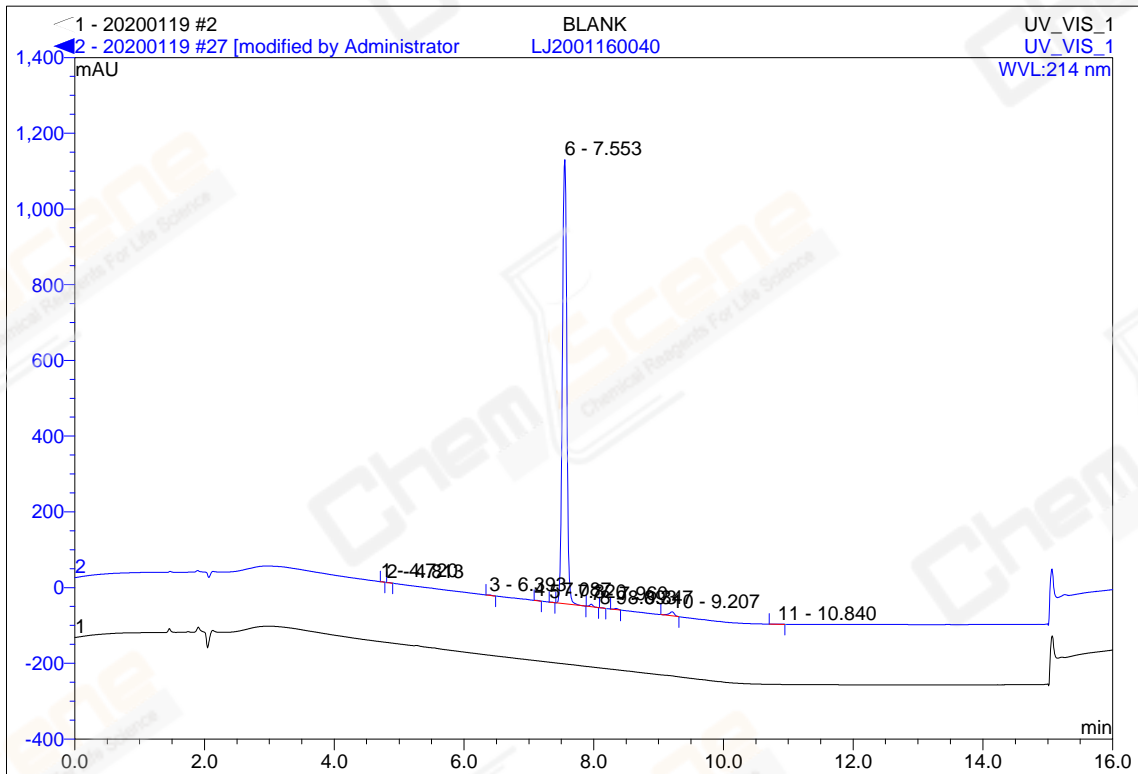

No.	Ret.Time min	Peak Name	Height mAU	Area mAU*min	Rel.Area %	Amount	Type
1	4.72	n.a.	0.038	0.017	0.02	n.a.	BMB*
2	4.81	n.a.	0.034	0.024	0.03	n.a.	BMB*
3	6.39	n.a.	1.053	0.059	0.06	n.a.	BMB*
4	7.09	n.a.	0.033	0.034	0.04	n.a.	BMB*
5	7.32	n.a.	0.002	0.016	0.02	n.a.	BMB*
6	7.55	n.a.	1173.360	93.290	98.10	n.a.	BMB*
7	7.96	n.a.	6.468	0.382	0.40	n.a.	BMB*
8	8.09	n.a.	0.078	0.025	0.03	n.a.	BMB*
9	8.35	n.a.	2.999	0.183	0.19	n.a.	BMB*
10	9.21	n.a.	10.727	1.035	1.09	n.a.	BMB*
11	10.84	n.a.	0.415	0.035	0.04	n.a.	BMB*
Total:			1195.206	95.099	100.00	0.000	