
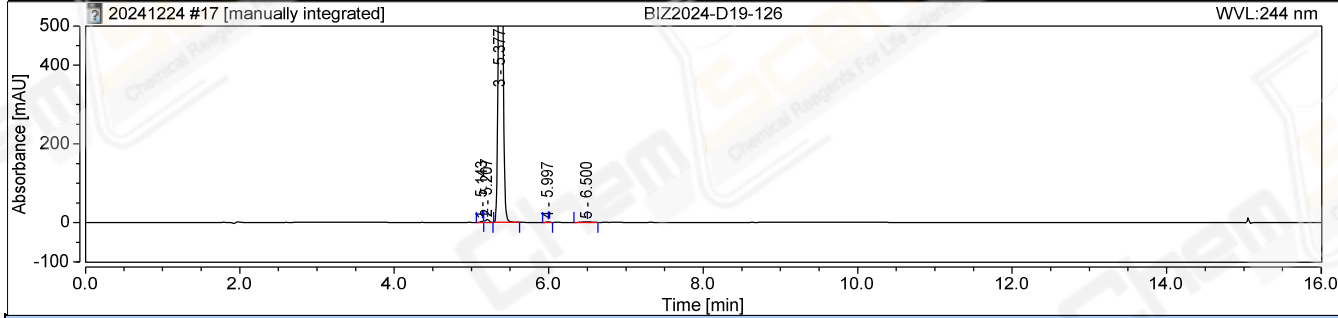


## Chromatogram and Results

Injection Details			
CAS NO.:	52-39-1	Run Time (min):	16.00
Vial Number:	RD5	Injection Volume:	2.00
Injection Type:	Unknown	Channel:	EXT244NM
Comment:	20241219-A-RP-1675	Wavelength:	n.a.
Instrument Method:	10-90A	Bandwidth:	n.a.
Processing Method:	3D Quantitative	Dilution Factor:	1.0000
Injection Date/Time:	24/Dec/24 16:02	seq.update_operator	GJH1472
seq.creation_operator	GJH1472	instMeth.creation_operator	GJH1472
injection.dilution_factor	1.0000	rdf.update_operator	GJH1472
instMeth.creation_time	19/Dec/2024 09:24		
chm.rawpath	chrom://thermo-hs/CDMO/2024/CSD/HPLC-35/Sequence/20241224.seq/969.smp/EXT244NM.channel/EXT244NM.chm		

### Chromatogram

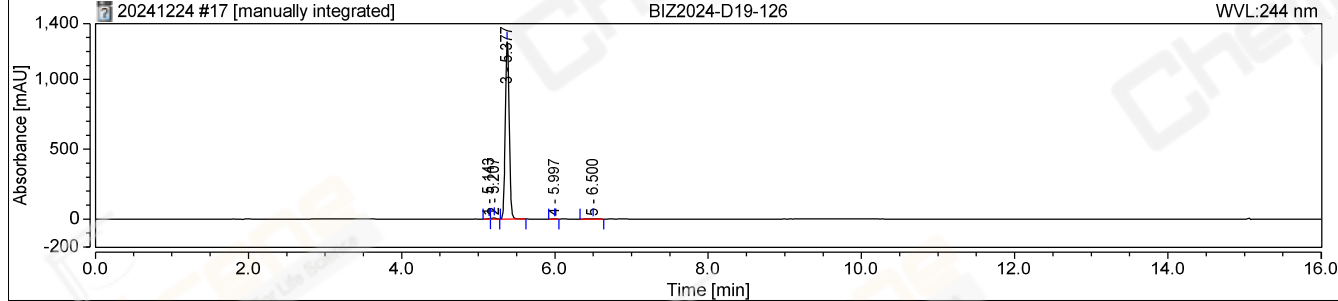

### Integration Results

No.	Peak Name	Retention Time min	Area mAU*s	Height mAU	Relative Area %	Resolution (USP)	Match	Plates (EP)
1		5.1433	8.3217	3.2206	0.1871	n.a.	972	n.a.
2		5.2067	26.5300	8.0190	0.5965	n.a.	989	55690
3		5.3767	4395.0436	1266.7500	98.8124	1.8703	1000	55262
4		5.9967	4.5039	1.4387	0.1013	6.9891	975	80623
5		6.5000	13.4662	1.5795	0.3028	3.2768	976	12830
<b>Total:</b>			<b>4447.8654</b>	<b>1281.008</b>	<b>100.0000</b>		<b>4912</b>	