


<b>24 LJ1912190012</b>			
<b>Catalog No : CS-W018811 Batch# Lc1219004 A-RP-243 JLW</b>			
Sample Name:	LJ1912190012	Injection Volume:	2.0
Vial Number:	GA2	Channel:	UV_VIS_1
Sample Type:	unknown	Wavelength:	214
Control Program:	10-90A 214NM	Bandwidth:	n.a.
Quantif. Method:	default	Dilution Factor:	1.0000
Recording Time:	2019-12-19 19:13	Sample Weight:	1.0000
Run Time (min):	16.00	Sample Amount:	1.0000

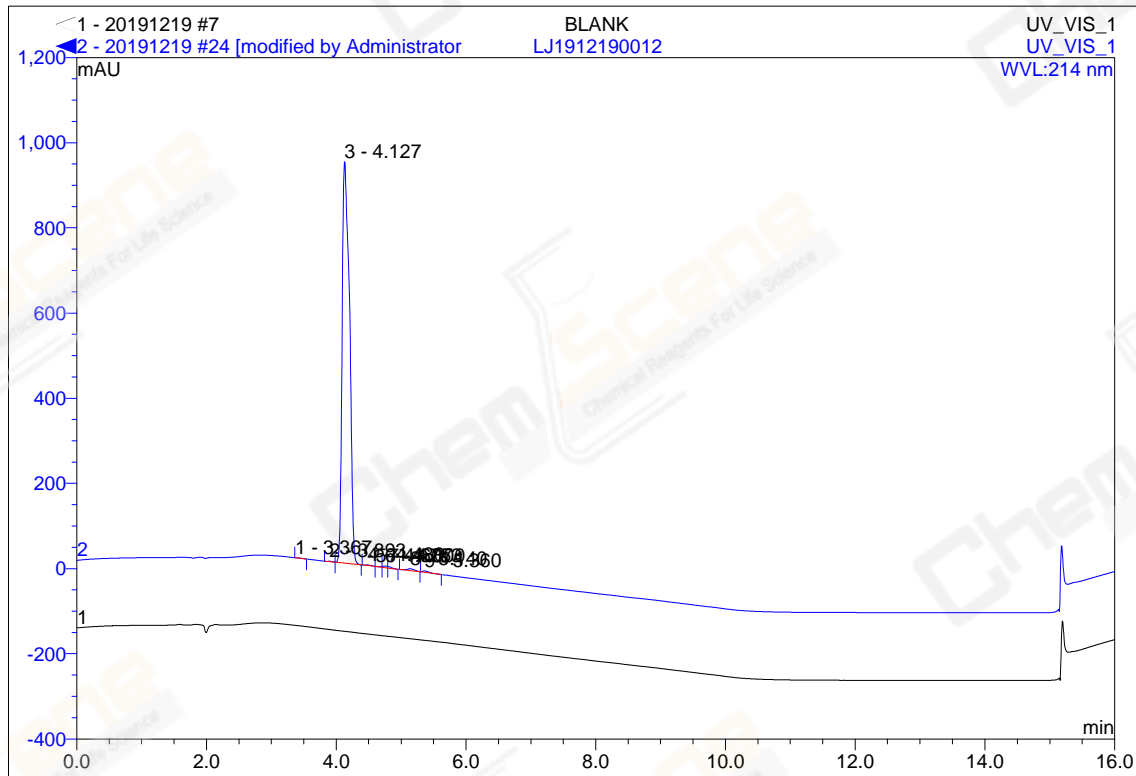

No.	Ret.Time min	Peak Name	Height mAU	Area mAU*min	Rel.Area %	Amount	Type
1	3.37	n.a.	0.008	0.044	0.04	n.a.	BMB*
2	3.89	n.a.	1.132	0.082	0.07	n.a.	BMb*
3	4.13	n.a.	942.586	122.717	98.53	n.a.	bMB*
4	4.48	n.a.	1.460	0.138	0.11	n.a.	BMb*
5	4.61	n.a.	0.022	0.079	0.06	n.a.	bM *
6	4.75	n.a.	4.095	0.292	0.23	n.a.	M *
7	4.80	n.a.	3.354	0.229	0.18	n.a.	MB*
8	5.14	n.a.	4.738	0.602	0.48	n.a.	BMB*
9	5.36	n.a.	3.465	0.359	0.29	n.a.	BMB
<b>Total:</b>			960.861	124.541	100.00	0.000	