
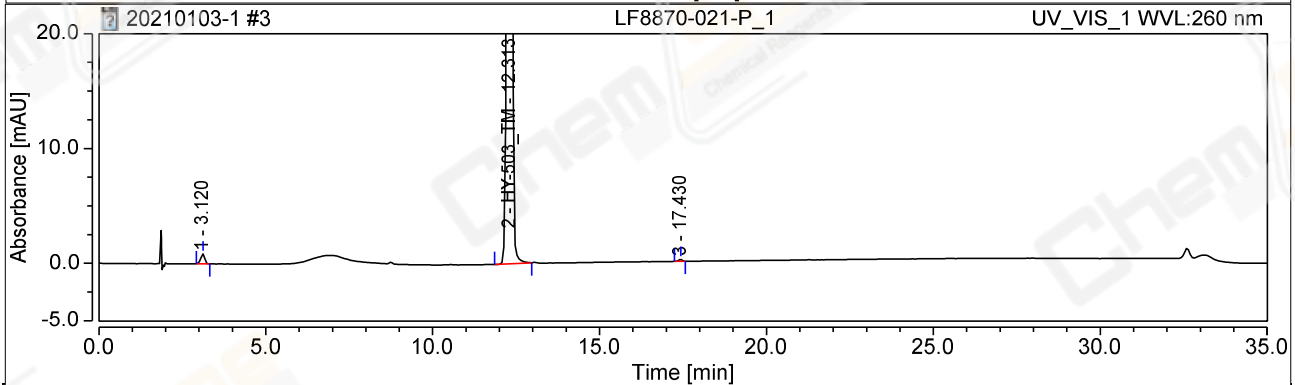


Chromatogram and Results

Injection Details

Injection Name: LF8870-021-P_1	Run Time (min): 35.00
Vial Number: R:B3	Injection Volume: 5.00
Injection Type: Unknown	Channel: UV_VIS_1
Comment: HY-503_TM-20210102 A-RP-490	Wavelength: 260
Instrument Method: HY-503_TM-H01RS01(RP-HPLC),A2B2	Bandwidth: 4
Processing Method: 10mM	Dilution Factor: 1.0000
Injection Date/Time: 03/Jan/21 12:01	Acq Operator: yrz

Chromatogram

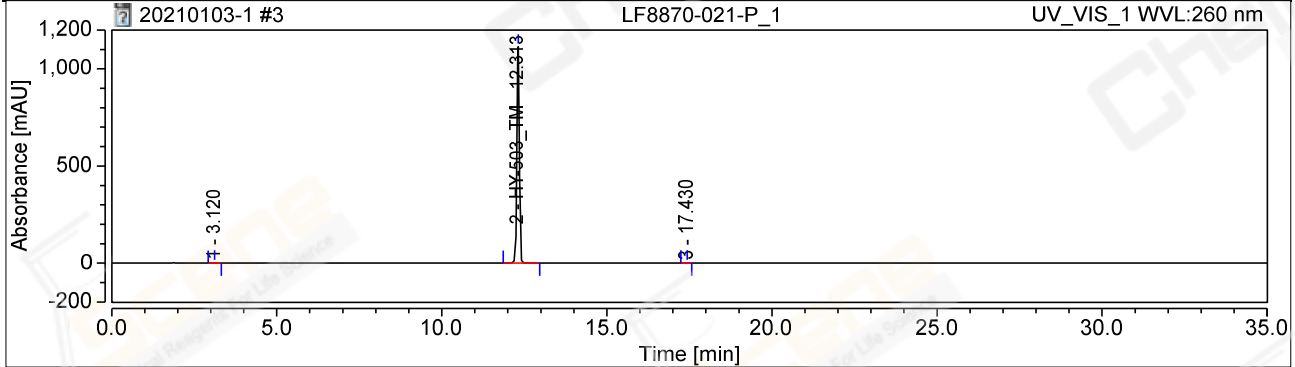

Integration Results



No.	Peak Name	Retention Time min	Area mAU*s	Height mAU	Relative Area %	Resolution	Plates	Asymmetry
1		3.120	7.1657	0.867	0.1285	53.06	3318	0.86
2	HY-503_TM	12.313	5566.9783	1113.396	99.8494	34.58	143843	0.96
3		17.430	1.2331	0.177	0.0221	n.a.	176222	0.93
Total:			5575.377	1114.441	100.00		323383.00	

Chromatogram and Results

Injection Details

Injection Name: LF8870-021-P_2	Run Time (min): 35.00
Vial Number: R:B4	Injection Volume: 5.00
Injection Type: Unknown	Channel: UV_VIS_1
Comment: HY-503_TM-20210102 A-RP-490	Wavelength: 260
Instrument Method: HY-503_TM-H01RS01(RP-HPLC),A2B2	Bandwidth: 4
Processing Method: 10mM	Dilution Factor: 1.0000
Injection Date/Time: 03/Jan/21 12:40	Acq Operator: yrz

Chromatogram

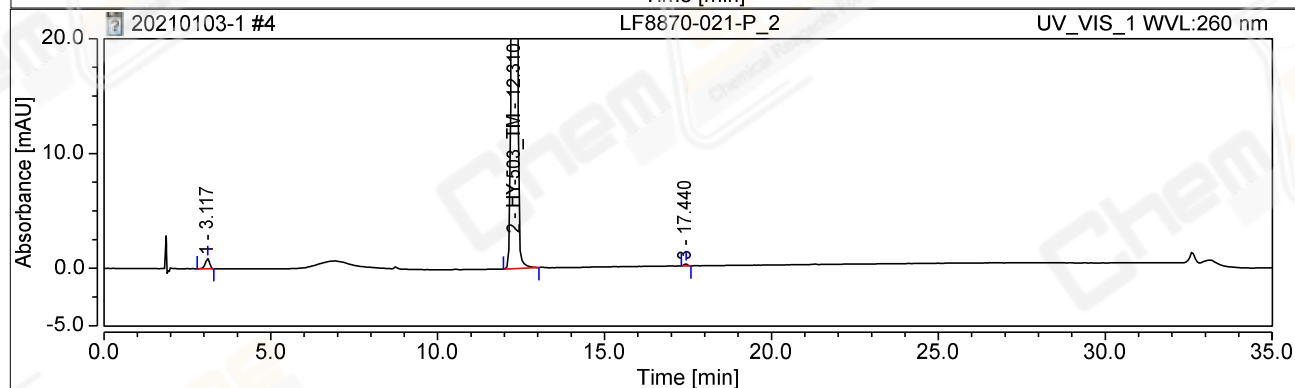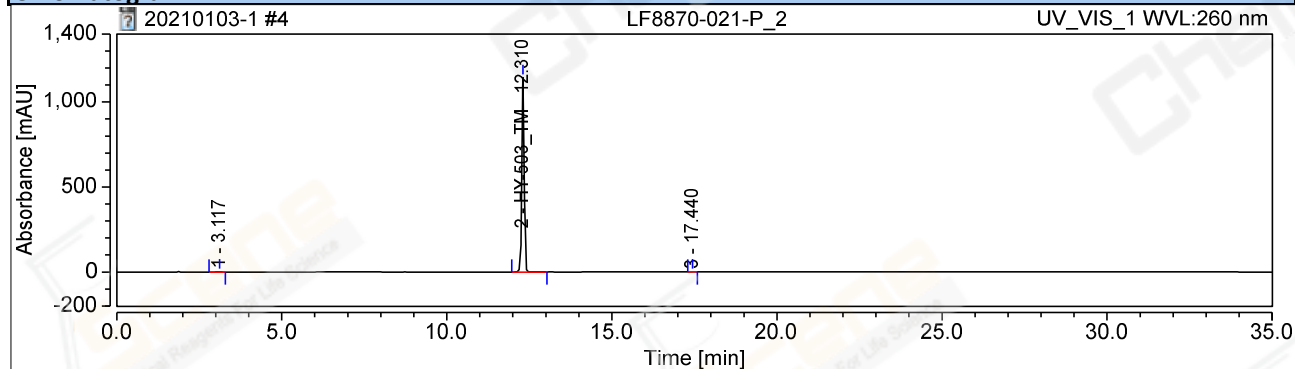

Integration Results

No.	Peak Name	Retention Time min	Area mAU*s	Height mAU	Relative Area %	Resolution	Plates	Asymmetry
1		3.117	7.7474	0.896	0.1351	51.57	3030	0.83
2	HY-503_TM	12.310	5724.7086	1143.616	99.8419	33.20	143345	0.97
3		17.440	1.3202	0.192	0.0230	n.a.	151943	0.99
Total:			5733.776	1144.703	100.00		298318.00	