


=====  
Acq. Operator : SYSTEM Seq. Line : 48  
Acq. Instrument : 7820A Location : 230 (B)  
Injection Date : 10/20/2020 7:59:32 PM Inj : 1  
Inj Volume : 1 µl  
Acq. Method : C:\Chem32\1\Data\00000 2020-10-20 09-05-44\20170719-280-.M  
Last changed : 10/20/2020 7:54:32 PM by SYSTEM  
(modified after loading)  
Analysis Method : C:\Chem32\1\Data\00000 2020-10-20 09-05-44\20170719-280-.M (Sequence Method  
Last changed : 10/21/2020 8:41:32 AM by SYSTEM  
(modified after loading)

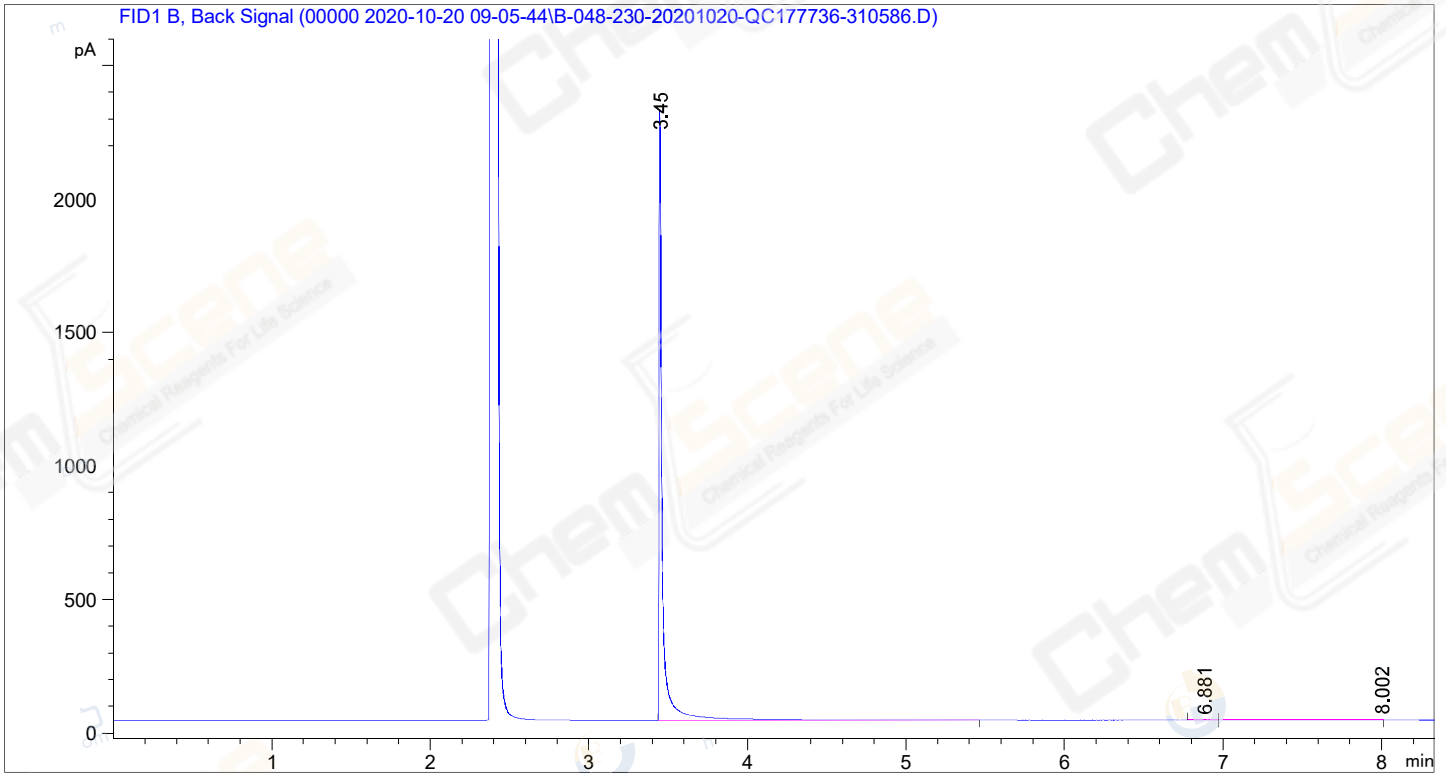

=====  
Area Percent Report  
=====

Sorted By : Signal  
Multiplier : 1.0000  
Dilution : 1.0000  
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: FID1 B, Back Signal

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Height [pA]	Area %
1	3.450	BB	0.0216	3311.43481	2191.30957	99.55068
2	6.881	BV	0.1105	3.15207	3.45143e-1	0.09476
3	8.002	VV	0.7365	11.79409	1.87597e-1	0.35456

Totals : 3326.38097 2191.84231

=====  
\*\*\* End of Report \*\*\*