
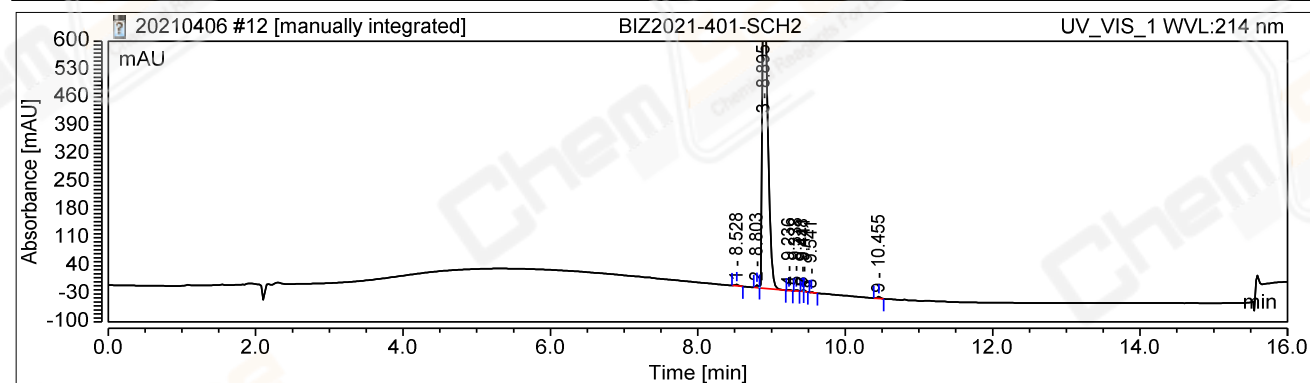


Chromatogram and Results

Injection Details

Injection Name: BIZ2021-401-SCH2
Vial Number: BA2
Injection Type: Unknown
Calibration Level:
Instrument Method: HY-119165-H01P01(RP-HPLC)
Processing Method: New Processing Method
Injection Date/Time: 06/Apr/21 16:07
CAS NO.: 884600-68-4 A-RP-541
Injection Volume: 5.00
Channel: UV_VIS_1
Wavelength: 214
Users: zx
Dilution Factor: 1.0000
Sample Weight: 1.0000
Run Time (min): 16.00
 chrom://hy261/Themo/Instrument Data/202104/20210406.seq/643.smp/UV_VIS_1.channel/UV_VIS_1.chm

Chromatogram

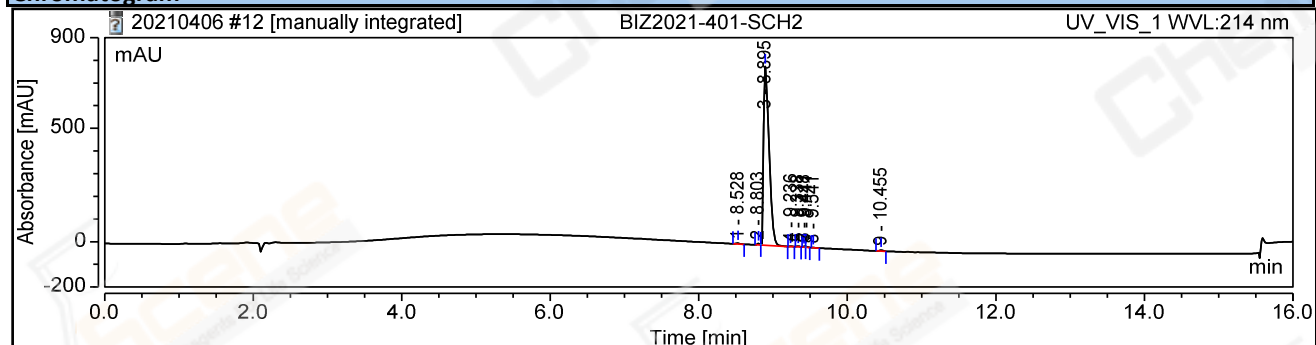

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Asymmetry (EP)	Plates (EP)	Rel.Area %
1		8.528	0.197	3.721	1.08	172198	0.29
2		8.803	0.250	6.363	n.a.	275534	0.37
3		8.895	66.547	788.235	2.16	66927	98.42
4		9.236	0.080	2.181	1.24	391144	0.12
5		9.338	0.106	2.991	1.13	420688	0.16
6		9.418	0.087	2.666	n.a.	n.a.	0.13
7		9.441	0.092	2.978	n.a.	n.a.	0.14
8		9.541	0.038	1.060	1.42	422403	0.06
9		10.455	0.222	4.845	1.00	329852	0.33

Total: 67.618 815.040 8.03