


10 LJ2018-0102-0001**Catalog No: CS-M1190 Batch#Lb0103011 A-RP-281 LHX**

Sample Name:	LJ2018-0102-0001	Injection Volume:	5.0
Vial Number:	RB6	Channel:	UV_VIS_1
Sample Type:	unknown	Wavelength:	214
Control Program:	10-90 214NM	Bandwidth:	n.a.
Quantif. Method:	default	Dilution Factor:	1.0000
Recording Time:	2018-1-2 13:34	Sample Weight:	1.0000
Run Time (min):	18.00	Sample Amount:	1.0000

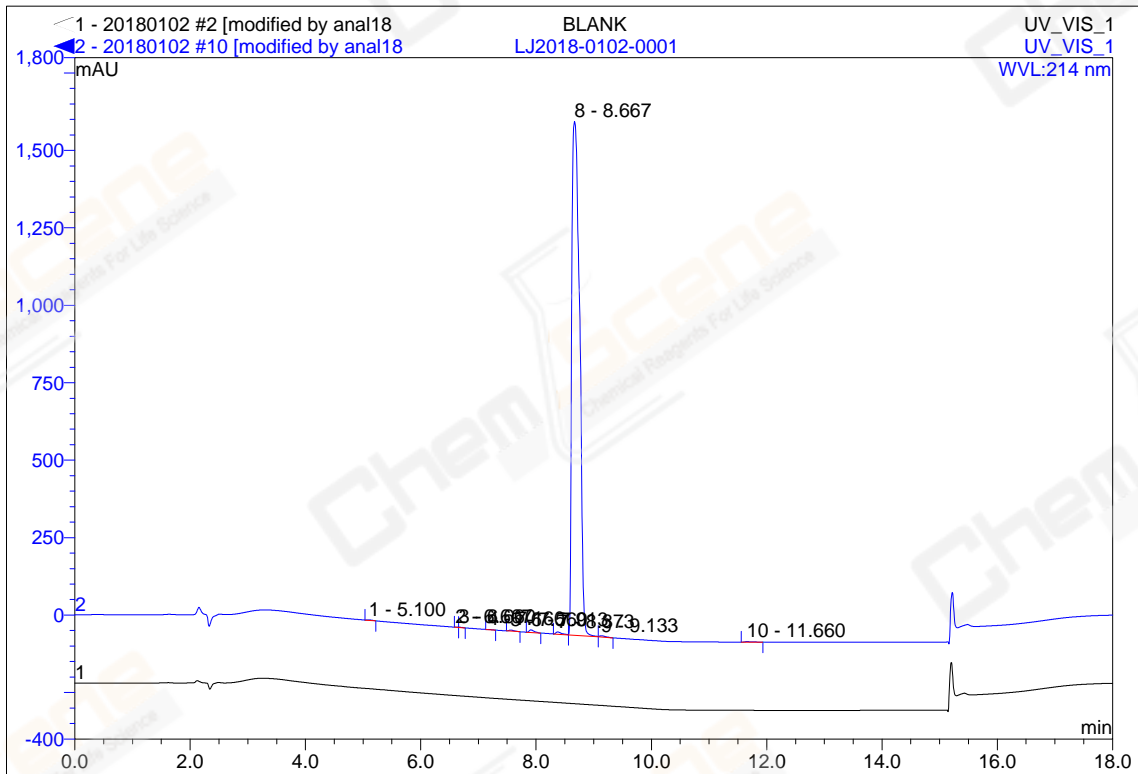

No.	Ret.Time min	Peak Name	Height mAU	Area mAU*min	Rel.Area %	Amount	Type
1	5.10	n.a.	1.590	0.161	0.06	n.a.	BMB*
2	6.61	n.a.	0.456	0.034	0.01	n.a.	BM *
3	6.66	n.a.	0.697	0.065	0.02	n.a.	MB*
4	7.16	n.a.	0.526	0.058	0.02	n.a.	BMB*
5	7.56	n.a.	3.544	0.354	0.13	n.a.	BMB*
6	7.91	n.a.	8.238	0.839	0.32	n.a.	BMB*
7	8.37	n.a.	7.195	0.834	0.32	n.a.	BM *
8	8.67	n.a.	1659.271	259.183	98.82	n.a.	M *
9	9.13	n.a.	4.225	0.524	0.20	n.a.	MB*
10	11.66	n.a.	1.353	0.227	0.09	n.a.	BMB*
Total:			1687.093	262.279	100.00	0.000	