


10 LJ2018-0104-0017			
Catalog No: CS-D1120 Batch#Lb0104016 A-RP-281 LHX			
Sample Name:	LJ2018-0104-0017	Injection Volume:	5.0
Vial Number:	RA7	Channel:	UV_VIS_1
Sample Type:	unknown	Wavelength:	214
Control Program:	10-90 214NM	Bandwidth:	n.a.
Quantif. Method:	default	Dilution Factor:	1.0000
Recording Time:	2018-1-5 19:45	Sample Weight:	1.0000
Run Time (min):	18.00	Sample Amount:	1.0000

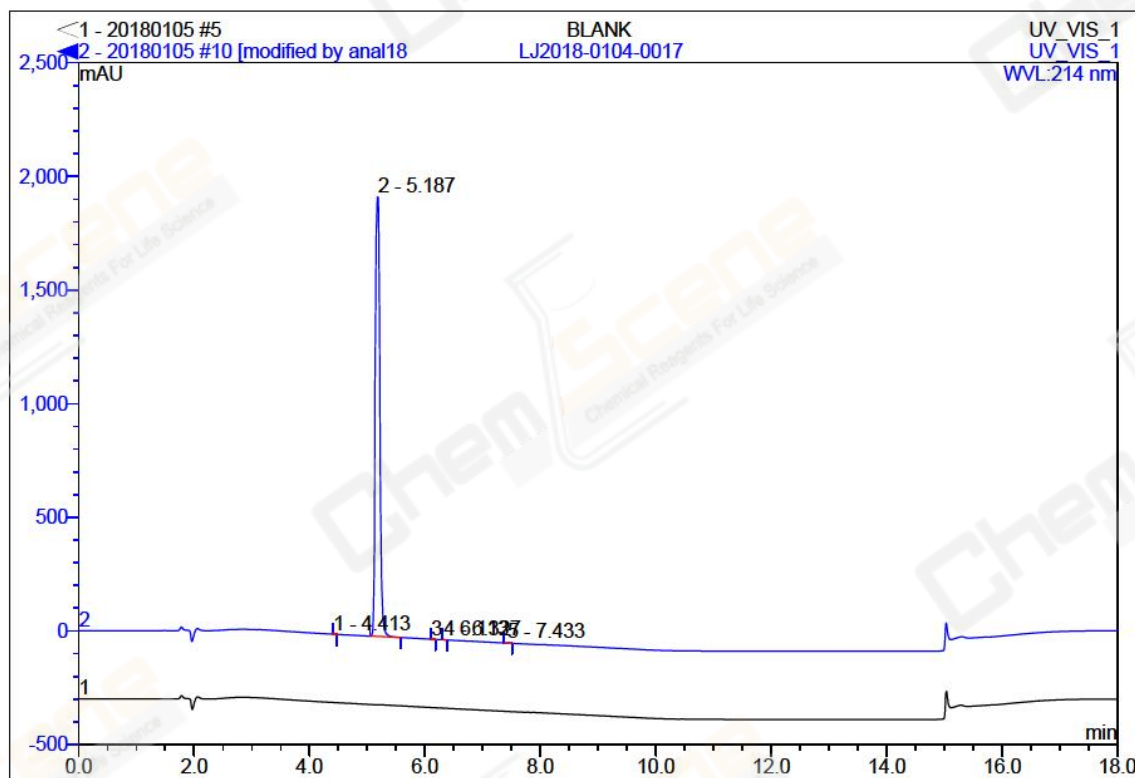

No.	Ret.Time min	Peak Name	Height mAU	Area mAU*min	Rel.Area %	Amount	Type
1	4.41	n.a.	0.053	0.012	0.01	n.a.	BMB*
2	5.19	n.a.	1935.305	177.163	99.90	n.a.	BMB*
3	6.11	n.a.	0.032	0.013	0.01	n.a.	BMB*
4	6.33	n.a.	0.592	0.027	0.02	n.a.	BMB*
5	7.43	n.a.	1.987	0.121	0.07	n.a.	BMB*
Total:			1937.970	177.335	100.00	0.000	