


Chromatogram and Results

Injection Details

Catalog No:	CS-W001157 Batch#Lc0305006	Injection Volume:	5.00
Vial Number:	GB1	Channel:	UV_VIS_1
Injection Type:	Unknown	Wavelength:	210
Calibration Level:		Users:	zqq
Instrument Method:	10-90A,214NM	Dilution Factor:	1.0000
Processing Method:	New Processing Method	Sample Weight:	1.0000
Injection Date/Time:	05/Mar/19 18:26	Run Time (min):	18.00
Comment:	A-RP -301	chrom://hy261/ChromeleonLocal/Chemistry Analy/201903/20190305.seq/635.smp/UV_VIS_1.channel/UV_VIS_1.chm	

Chromatogram

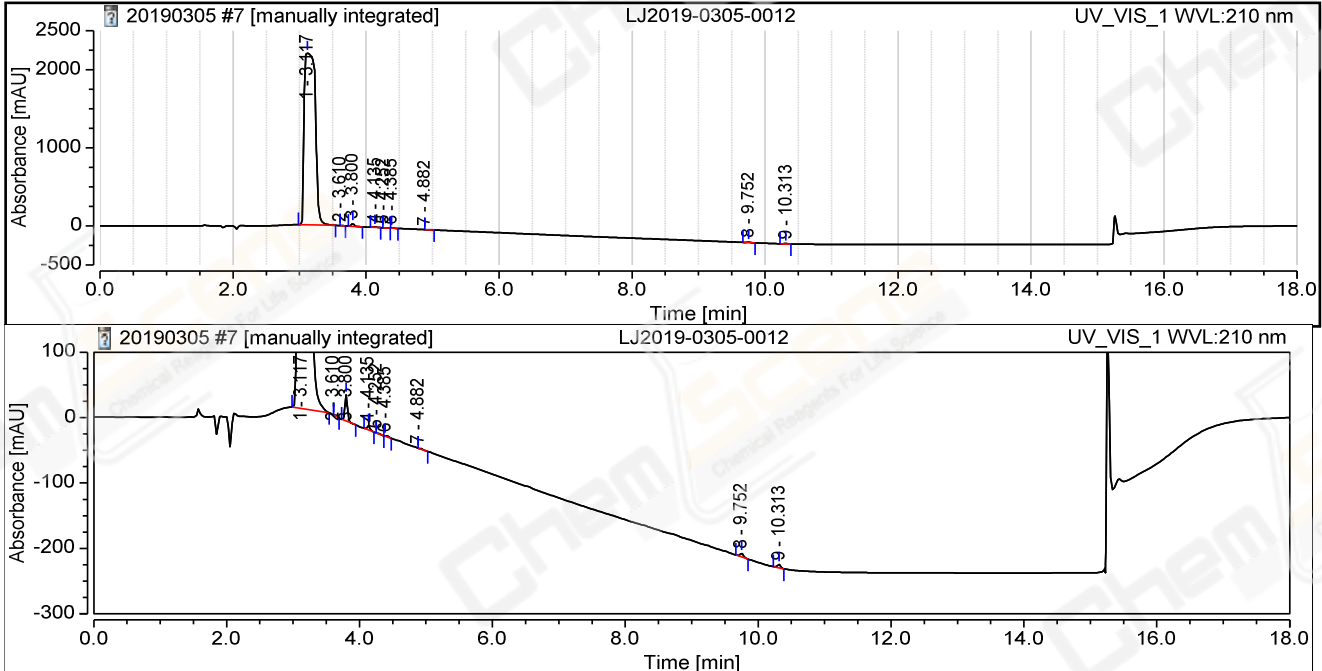

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Asymmetry (EP)	Resolution (EP)	Rel.Area %
1		3.117	418.139	2198.250	1.85	n.a.	99.33
2		3.610	0.066	0.000	n.a.	n.a.	0.02
3		3.800	1.675	39.989	1.06	4.98	0.40
4		4.135	0.297	6.528	1.19	n.a.	0.07
5		4.252	0.030	0.000	n.a.	n.a.	0.01
6		4.385	0.098	0.946	3.41	n.a.	0.02
7		4.882	0.057	0.000	n.a.	n.a.	0.01
8		9.752	0.317	5.783	1.05	6.64	0.08
9		10.313	0.290	5.416	0.99	n.a.	0.07
Total:			420.969	2256.911	9.55	11.62	