


13 LJ1909170104**Catalog No: CS-D0718 Batch#Lc0917064 A-RP-243 JLW**

Sample Name:	LJ1909170104	Injection Volume:	5.0
Vial Number:	BA4	Channel:	UV_VIS_1
Sample Type:	unknown	Wavelength:	214
Control Program:	10-90A 214NM	Bandwidth:	n.a.
Quantif. Method:	default	Dilution Factor:	1.0000
Recording Time:	2019-9-19 19:02	Sample Weight:	1.0000
Run Time (min):	16.00	Sample Amount:	1.0000

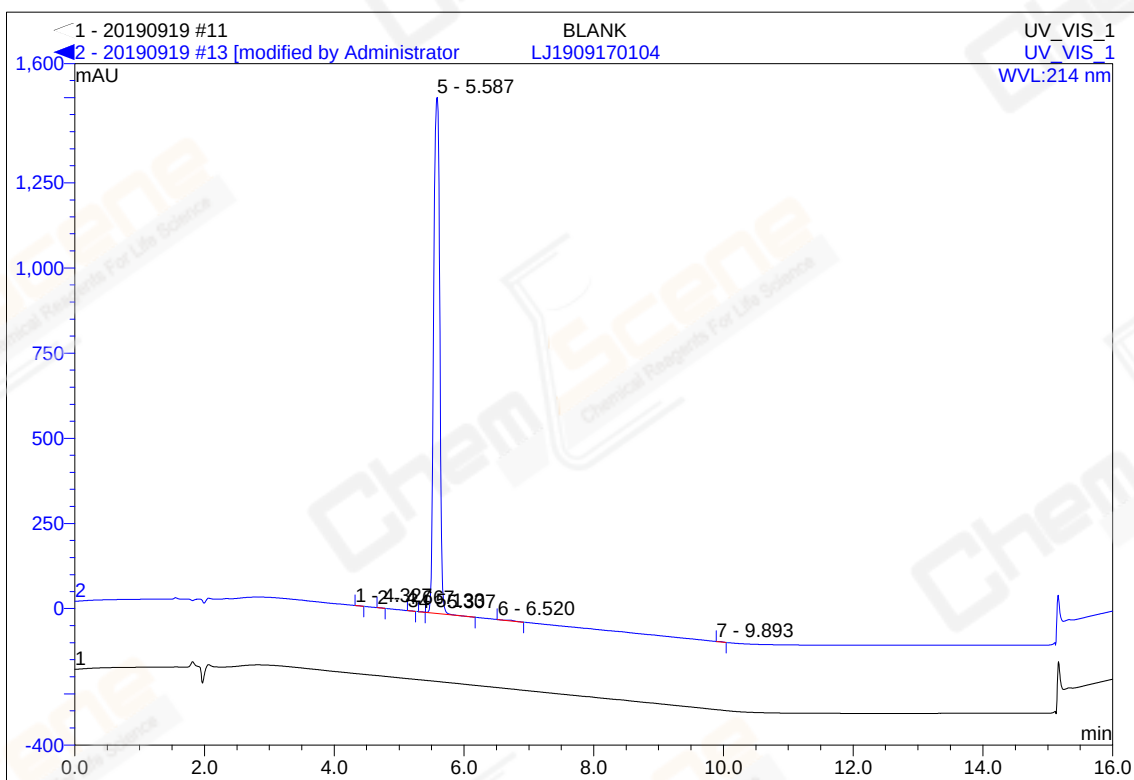

No.	Ret.Time min	Peak Name	Height mAU	Area mAU*min	Rel.Area %	Amount	Type
1	4.33	n.a.	0.000	0.025	0.02	n.a.	BMB*
2	4.67	n.a.	0.031	0.026	0.02	n.a.	BMB*
3	5.13	n.a.	0.017	0.020	0.01	n.a.	BMB*
4	5.31	n.a.	0.036	0.022	0.01	n.a.	BMB*
5	5.59	n.a.	1514.687	160.693	99.78	n.a.	BMB
6	6.52	n.a.	0.003	0.194	0.12	n.a.	BMB
7	9.89	n.a.	0.049	0.064	0.04	n.a.	BMB*
Total:			1514.823	161.043	100.00	0.000	